
ABB MEASUREMENT & ANALYTICS | DATA SHEET

CoriolisMaster FCB100, FCH100

Coriolis mass flowmeter



Measurement made easy

Compact device for high-precision measurement of mass and volume flow, density, temperature and concentration with just one device

The ideal transmitter for system integration

- Modbus for quick and comprehensive communication
- Two fast digital outputs that can be configured as pulse outputs, frequency outputs or binary outputs
- Lower pressure loss, self-draining
- Global approvals for explosion protection
- MID / OIML approval for legal metrology

Integrated VeriMass device verification and diagnosis

- Predictive maintenance in the process
- Extended maintenance cycles
- Reduced maintenance effort

CoriolisMaster Software Tools

- DensiMass for concentration measurements, net mass and volume flow calculations
- FillMass for filling applications

CoriolisMaster FCH100

- For hygienic applications

Overview – models

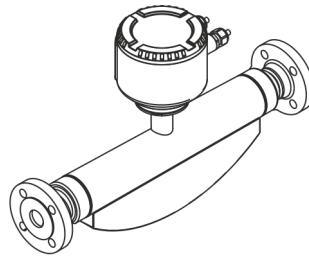


Figure 1: FCB1xx/FCH1xx

Model number	FCB1xx for standard applications	FCH1xx for hygienic applications
Process connections		
Flange DIN 2501 / EN 1092-1	DN 10 to 200, PN 40 to 100	—
Flange ASME B16.5	DN ½ to 8 in, CL150 to CL1500	—
JIS flange	DN 10 to 200; JIS 10K to 20K	—
Pipe fitting DIN 11851	DN 10 to 100 (¼ to 4 in)	DN 15 to 100 (½ to 4 in)
Pipe fitting SMS 1145	DN 25 to 80 (1 to 3 in)	—
Tri-clamp DIN 32676 (ISO 2852)	DN 15 to 100 (¼ to 4 in)	DN 20 to 100 (¼ to 4 in)
Tri-clamp BPE	DN ¾ to 4 in	DN ¾ to 4 in
Female thread DIN ISO 228 and ASME B 1.20.1	DN 15; PN 100	—
Other connections	On request	On request
Wetted material		
	Stainless steel 1.4435 or 1.4404 (AISI 316L), nickel alloy C4 / C22	Stainless steel, polished 1.4404 (AISI 316L) or 1.4435 (AISI 316L)
Approvals and certificates		
Explosion protection	Zone 0, 1, 2, 21, 22	Zone 0, 1, 2, 21, 22
ATEX, IECEx, UKEX, EAC-Ex	—	—
Explosion protection conforming to cFMus	Class I Div. 1, Class I Div. 2, Zone 0, 1, 2, 21	Class I Div. 1, Class I Div. 2, Zone 0, 1, 2, 21
Hygiene approvals	—	FDA compliant
Legal metrology	OIML R117, MID, devices for legal metrology in accordance with API / AGA	—
Additional approvals	Available from www.abb.com/flow or upon request.	

... Overview – models

... Device description

Model number	FCB130	FCB150	FCH130	FCH150
Measuring accuracy for liquids				
Mass flow*	0.4 %, 0.25 % and 0.2 %	0.1 % and 0.15 %	0.4 %, 0.25 % and 0.2 %	0.1 % and 0.15 %
Volume flow*	0.4 %, 0.25 % and 0.2 %	0.15 % and ± 0.11 %	0.4 %, 0.25 % and 0.2 %	0.15 % and ± 0.11 %
Density	0.01 kg/l	<ul style="list-style-type: none"> • 0.002 kg/l • 0.001 kg/l (optional) • 0.0004 kg/l (optional) 	0.01 kg/l	<ul style="list-style-type: none"> • 0.002 kg/l • 0.001 kg/l (optional) • 0.0004 kg/l (optional)
Temperature	1 K	0,5 K	1 K	0,5 K
Measuring accuracy for gases*				
Permissible measuring medium temperature	-50 to 160 °C (-58 to 320 °F)	-50 to 205 °C (-58 to 400 °F)	-50 to 160 °C (-58 to 320 °F)	-50 to 205 °C (-58 to 400 °F)
Permissible ambient temperature	-40 to 70 °C (-40 to 158 °F)			
Power supply	11 to 30 V DC, nominal voltage: 24 V DC			
IP rating in accordance with EN 60529	IP 65 / IP 67 / IP 68 (immersion depth: 5 m), NEMA 4X			
Communication	Modbus® RTU, RS485			
Outputs in serial production	<ul style="list-style-type: none"> • Digital output 1: passive • Digital output 2: passive 			
External output zero return	Yes			
External totalizer reset	Yes			
Flow measurement in forward flow and reverse flow direction	Yes			
Empty pipe detection	Yes, based on preconfigured density alarm			
Self-monitoring and diagnosis	Yes			
Field optimization for flow and density	Yes			
Concentration measurement 'DensiMass'	Yes, optional on models FCB150 and FCH150			
'FillMass' filling function	Yes, optional on models FCB150 and FCH150			
"VeriMass" diagnosis function	Yes, optional			

* Indication of accuracy in % of the measured value (% of meas.val.)

General data

Device description

The CoriolisMaster FCB100, FCH100 is the low-cost and simple ABB mass flowmeter with the new DSP transmitter.

The device is equipped with a Modbus® interface and two fast digital outputs that can be configured as pulse, frequency or binary outputs.

The CoriolisMaster FCB100, FCH100 operates in accordance with the Coriolis principle. The design offers the following benefits:

- Space-saving, robust design.
- Variety of process connections.
- Two digital outputs.
- Communication viaModbus® RTU protocol.
- Ex approval The user can select the "i" or "e" type of protection for the output circuits; the type chosen will depend on the circuits which are connected. The type of protection can be changed even after installation has been completed.

... General data

FillMass batch function

Only for FCB150 / FCH150

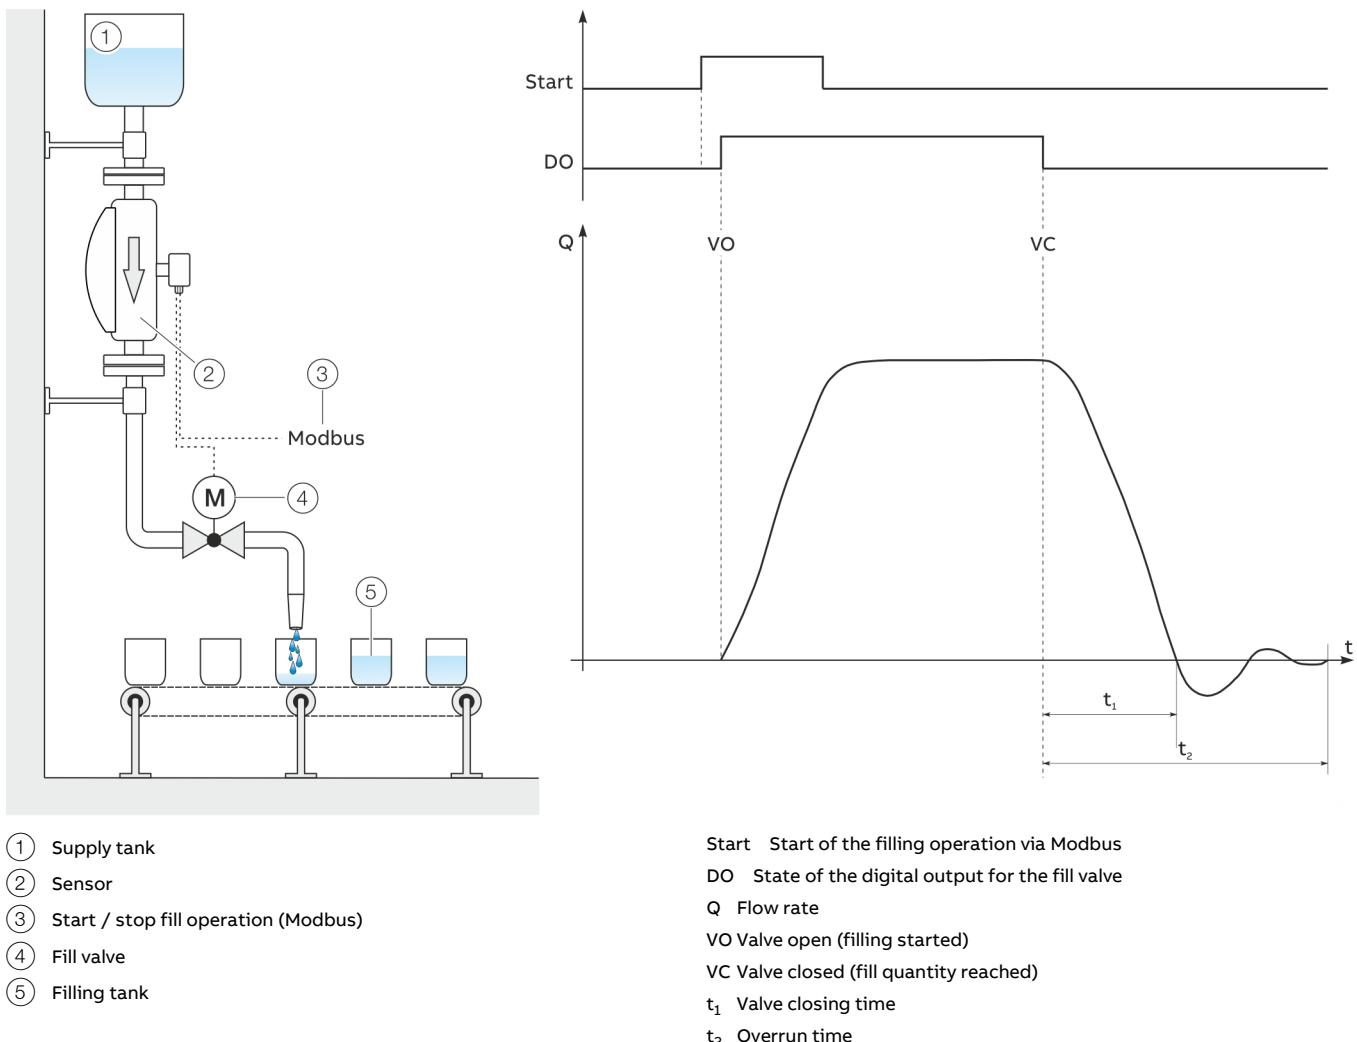


Figure 2: FillMass fill function

The integrated FillMass fill function allows filling operations with filling times of > 3 s.

For this purpose, the filling quantity is given via an adjustable totalizer.

The Modbus interface is used to configure and control the fill function.

The valve is triggered via one of the digital outputs and closed again once the preset filling quantity is reached.

The transmitter measures the overrun quantity and calculates the overrun correction from this.

Additionally, the low flow cut-off can be activated if required.

Concentration measurement DensiMass

Only for FCB150 / FCH150

The transmitter can calculate the current concentration from the measured density and temperature using concentration matrices.

The following concentration matrices are preconfigured in the transmitter as standard:

- Concentration of sodium hydroxide in water
- Concentration of alcohol in water
- Concentration of sugar in water
- Concentration of maize starch in water
- Concentration of wheat starch in water
- Concentration of antifreeze in water

In addition, the user can enter two user-defined matrices:

- Up to 100 values with one matrix
- Up to 50 values per matrix with two matrices

Calculating standard volumes and standard densities of liquids

If a suitable matrix is available, the DensiMass function also allows the measured volume to be corrected for any selected temperature.

The measured density can also be corrected for a given temperature.

However, this is only possible when measuring liquids and after entering an appropriate matrix.

This correction can also be performed using the default matrices (see above).

The calculated standard volumes and standard densities can also be issued for all other process variables.

The software 'DensiMatrix' is available for the easy input of the matrix.

Accuracy of the concentration measurement

The accuracy of the concentration measurement is determined in the first instance by the quality of the matrix data entered.

However, as the calculation is based on temperature and density (the input variables), the accuracy of the concentration measurement is ultimately determined by the measuring accuracy of the temperature and the density.

Example:

Density of 0 % alcohol in water at 20 °C (68 °F): 998.23 g/l

Density of 100 % alcohol in water at 20 °C (68 °F): 789.30 g/l

Concentration	Density
100 %	208.93 g/l
0.48 %	1 g/l
0.96 %	2 g/l
0.24 %	0.5 g/l

Thus, the accuracy class of the density measurement directly determines the accuracy of the concentration measurement.

... General data

Enhanced Coriolis Control (ECC)function

The Enhanced Coriolis Control (ECC)function has been specially developed for demanding applications, such as:

- Liquids with gas phase
- Liquids with rapidly changing densities
- Fill operations with surge phases at the beginning or end
- Liquids with high viscosity

After the ECC function is activated, the device applies a particularly quick control algorithm to control the oscillating tubes in the device and therefore provide significantly better behavior in the applications listed above.

In addition, the ECC function offers a special noise suppression filter for mass flow measurement and density measurement.

In the case of particularly demanding applications, disruptions can thus be actively filtered and the measurement can be implemented in a considerably more stable manner.

For the filters, a variety of time constants between 0.5 s and 8 s can be selected.

Since Coriolis mass flowmeters measure the mass flow and density separately, the CoriolisMaster features a separate filter each for mass flow measurement and density measurement.

Devices for legal metrology in accordance with MID / OIML R117

The Coriolis mass flowmeters CoriolisMaster FCBx50 are type-tested for legal metrology in accordance with MID / OIML R117 in accuracy classes 0.5 and 0.3.

Additional information can be found on the corresponding certificate. The certificate is available in the download area at www.abb.com/flow.

When ordering, select one of the optional order codes:

- CT4 – Approved for official calibration in accordance with MID (OIMLR117 Cl0.5)
- CT3 – Approved for official calibration in accordance with MID (OIMLR117 Cl0.5/0.3)

All Coriolis mass flowmeters FCBx50 for legal metrology receive a 3-point flow rate calibration at the factory, which demonstrates measuring accuracy in accordance with the OIML-R117-2019 guidelines at minimum (Q_{\min}), medium and maximum (Q_{\max}) flow rates.

Nominal diameter	Q1 (tol. +10 %) [kg/h]	Q2 (tol. ±10 %) [kg/h]	Q3 (tol. -20 %) [kg/h]
DN 15	365	2489	6500
DN 25	1620	10570	27000
DN 50	4550	27335	67000
DN 80	14500	91489	145000
DN 100	23000	124597	290000
DN 150	32000	178053	290000*

* corresponds to approx. 60 % $Q_{\max}CT$

Note

Use in accordance with API / AGA standards is also possible.

Please observe the additional remarks in the operating and commissioning instruction.

Applications in accordance with API (American Petroleum Institute)

For applications in accordance with API Chapter 5.6, the CoriolisMaster FCB100, FCH100 provides special parameters:

- Calibration Pressure: Measuring medium pressure at which the device was calibrated at ABB.
- Calibration Temp.: Measuring medium temperature at which the device was calibrated at ABB.
- Pressure Level: Parameters for entry of the current operating pressure in the device by the user.
- Flow Compens. factor: Display / output of the current compensation factor for mass flow calculation.
- Density Comp. factor: Display / output of the current compensation factor for density calculation.
- P.Comp.Status (PECI): In accordance with API, the user can set the following states:
 - 1: CT: Compensation in the Coriolis flowmeter based on the current pressure entered in the 'Pressure Level' parameter.
 - 2: TD: Compensation in the Coriolis flowmeter switched off – compensation is performed externally (Tertiary Device)
 - 3: OS: Compensation in the Coriolis flowmeter switched off – compensation is not performed on site (Off Site)
 - 4: NA: Compensation in the Coriolis flowmeter switched off – compensation is not deemed to be necessary, since the device is operating at a pressure for which the device has been proved.

VeriMass erosion monitor

The integrated diagnosis function VeriMass allows the status of the meter tube to be monitored. This enables changes due to material erosion and the formation of deposits on the meter tube walls to be identified at an early stage.

If the set limit value is exceeded, an alarm is triggered, for example via the programmable digital output or HART, depending on the configuration.

The limit value for the erosion monitor can be set either automatically or manually.

Automatic adjustment

The transmitter monitors the sensor's driver current over a prolonged period and creates a 'fingerprint' for the relevant application. The transmitter generates a corresponding tolerance value for deviations in the driver current.

The transmitter compares the behavior of the driver current with the generated fingerprint and triggers the relevant error message in the event of prolonged deviations.

Manual adjustment

For applications where automatic adjustment of the erosion monitor does not provide a satisfactory result, the erosion monitor can be adjusted manually.

For more information, please contact ABB Service or the sales organization.

Flowmeter sensor

General installation conditions

Installation location and assembly

Note the following points when selecting the installation location and when mounting the sensor:

- The ambient conditions (IP rating, ambient temperature range T_{ambient}) of the device must be adhered to at the installation location.
- Sensors and transmitters must not be exposed to direct sunlight. If necessary, provide a suitable means of sun protection on site. The limit values for ambient temperature T_{ambient} must be adhered to.
- On flange devices, ensure that the counterflanges of the piping are aligned plane parallel. Only install flange devices with suitable gaskets.
- Prevent the sensor from coming into contact with other objects.
- The device is designed for industrial applications. No special EMC protective measures are required if the electromagnetic fields and interference at the installation location of the device comply with 'Best Practice' (in accordance with the standards listed in the declaration of conformity).

Maintain a suitable distance from electromagnetic fields and interference that extend beyond the usual dimensions.

Seals

Users are responsible for selecting and mounting suitable gaskets (material, shape).

Note the following points when selecting and mounting gaskets:

- Use gaskets made from a material that is compatible with the measuring medium and measuring medium temperature.
- Gaskets must not extend into the flow area, since possible turbulence may influence the accuracy of the device.

Calculating pressure loss

Pressure loss depends on the properties of the medium and the flow rate.

A good aid for pressure loss calculation is the Online ABB Product Selection Assistant (PSA) for flow at www.abb.com/flow-selector.

Brackets and supports

No special supports or damping are required for the device when the device is used and installed as intended.

In systems designed in accordance with 'Best Practice', the forces acting on the device are already sufficiently absorbed. This is also true of devices installed in series or in parallel. For heavier devices, it is advisable to use additional supports / brackets on site. Doing this prevents damage to the process connections and piping from lateral forces.

Please observe the following points:

- Mount two supports or brackets symmetrically in the immediate vicinity of the process connections.
- Do not fasten any supports or brackets to the housing of the flowmeter sensor.

Note

For increased vibration load, such as for example on ships, the use of the 'CL1' marine design is recommended.

Inlet section

The sensor does not require any inlet section.

The devices can be installed directly before/after manifolds, valves or other equipment, provided that no cavitation is caused by this equipment.

Mounting position

The flowmeter operates in any mounting position.

Depending on the measuring medium (liquid or gas) and the measuring medium temperature, certain mounting positions are preferable to others. For this purpose, consider the following examples.

The preferred flow direction is indicated by the arrow on the sensor. The flow will be displayed as positive.

The specified measuring accuracy can be achieved only in the calibrated flow direction (for forward flow calibration, this is only in the direction of the arrow; for the optional forward flow and reverse flow calibration, this can be in both flow directions).

Liquid measuring media

Observe the following points to avoid measuring errors:

- The meter tubes must always be completely filled with the measuring medium.
- The gases dissolved in the measuring medium must not leak out. To safeguard this, a minimum back pressure of 0.2 bar (2.9 psi) is recommended.
- The minimum vapor pressure of the measuring medium must be maintained when there is negative pressure in the meter tube or when liquids are gently simmering.
- During operation, there must be no phase transitions in the measuring medium.

Vertical installation

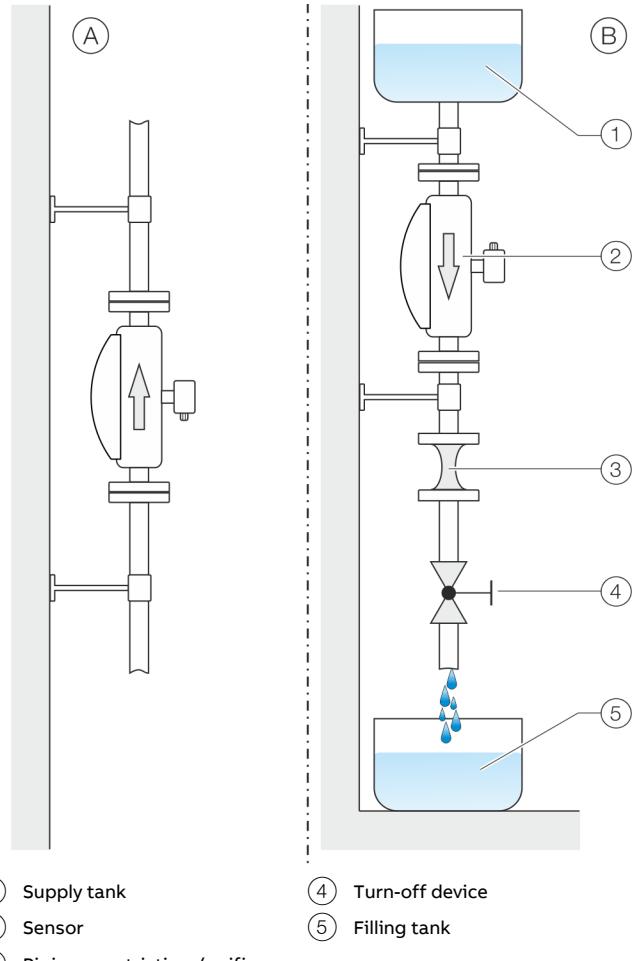


Figure 3: Vertical installation

- (A) For vertical installation in a riser, no special measures are required.
- (B) For vertical installation in a downpipe, a piping constriction or an orifice must be installed below the sensor. Doing this prevents the sensor from draining during the measurement.

Horizontal installation

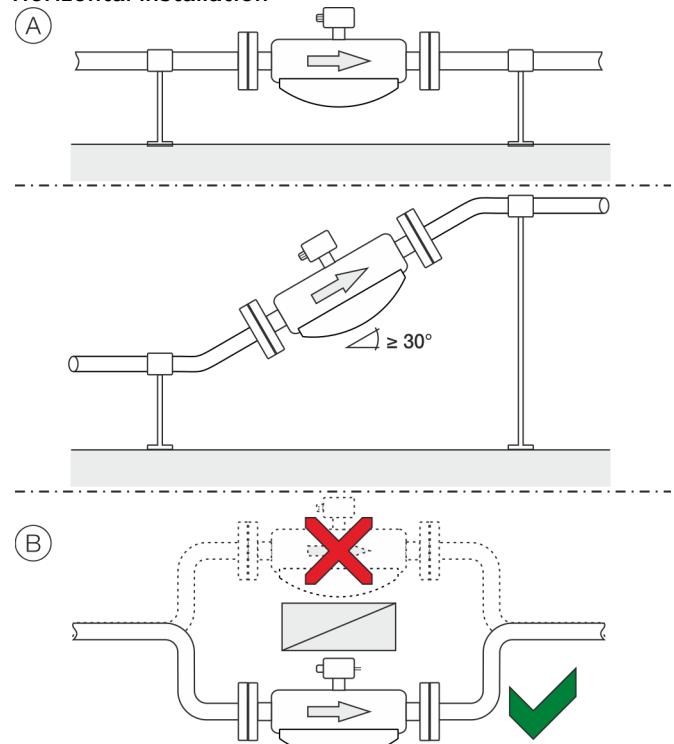


Figure 4: Horizontal installation

- (A) For liquid measuring media and horizontal installation, the transmitter and terminal box must point upward. If a self-draining installation is required, the sensor must be mounted at an incline of $\geq 30^\circ$.
- (B) Installing the sensor at the highest point of the piping leads to an increased number of measuring errors due to the accumulation of air or the formation of gas bubbles in the meter tube.

... Flowmeter sensor

... General installation conditions

Gaseous measuring media

Observe the following points to avoid measuring errors:

- Gases must be dry and free of liquids and condensates.
- Avoid the accumulation of liquids and the formation of condensate in the meter tube.
- During operation, there must be no phase transitions in the measuring medium.

If there is a risk of condensate formation when using gaseous measuring media, note the following:

Ensure that condensates cannot accumulate in front of the sensor.

If this cannot be avoided, we recommend that the sensor is installed vertically with a downward flow direction.

Vertical installation

For vertical installation, no special measures are required.

Horizontal installation



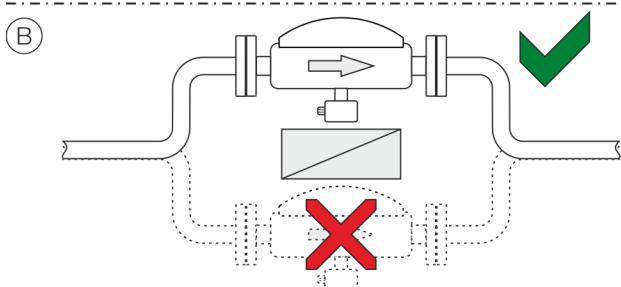


Figure 5: Horizontal installation

- (A) For gaseous measuring media and horizontal installation, the transmitter and terminal box must point downward.
- (B) Installing the sensor at the lowest point of the piping leads to an increased number of measuring errors due to the accumulation of liquid or the formation of condensates in the meter tube.

Turn-off devices for the zero point adjustment

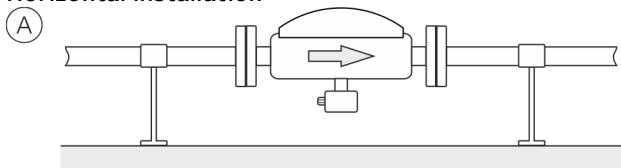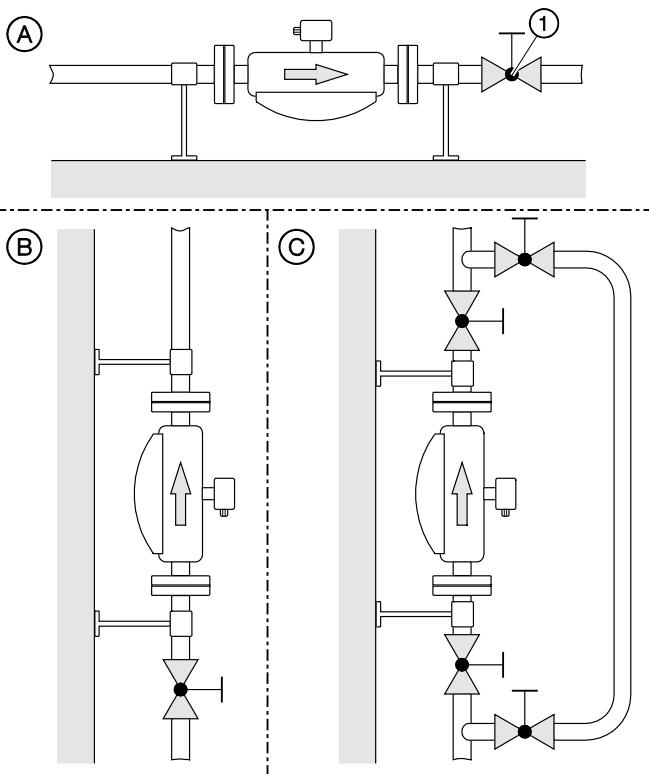


(1) Turn-off device

Figure 6: Mounting options for turn-off devices (example)

To guarantee the conditions for zero point balancing under operating conditions, turn-off devices are required in the piping:

- (A) At least on the outlet side when the transmitter is mounted in horizontal position
- (B) At least on the inlet side when the transmitter is mounted in vertical position.
- (C) In order to perform balancing during an ongoing process, it is advisable to mount a bypass pipe.

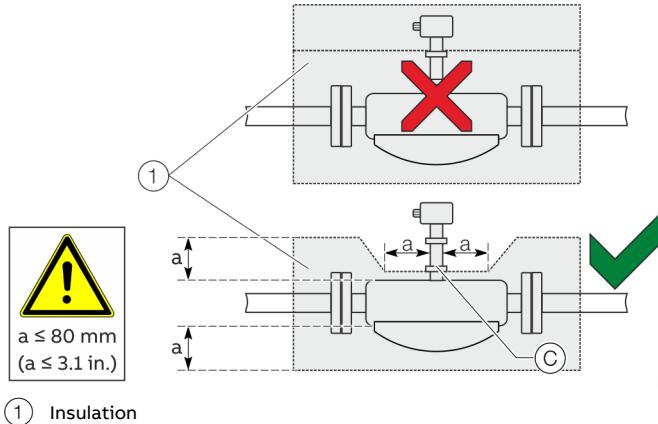Sensor insulation

The sensor may only be insulated in conjunction with the option TE1 'Extended tower length for sensor insulation' or TE2 'Extended tower length – insulation capacity with dual gasket,' as shown in Figure 7.

Heat tracing of the sensor

When operating the sensor in conjunction with heat tracing, the temperature at point (C) (Figure 7) 100°C (212°F) may not be exceeded at any time!

Installation in EHEDG-compliant installations**WARNING****Risk of poisoning!**

Bacteria and chemical substances can contaminate or pollute pipeline systems and the materials they are made of.

- In EHEDG-compliant installations, the instructions below must be observed.

- The required self-draining functionality of the sensor can only be guaranteed when the vertical mounting position or horizontal mounting position at a 30° incline is used. Refer to **Liquid measuring media** on page 11.
- The combination of process connections and gaskets selected by the operator may comprise only EHEDG-compliant components. Please note the information in the latest version of the EHEDG Position Paper: 'Hygienic Process connections to use with hygienic components and equipment' in this regard.

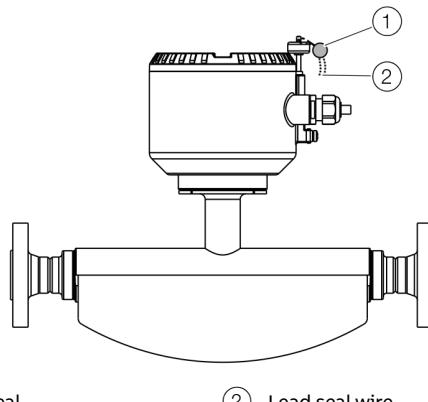
Devices for legal metrology

Figure 8: Sealing in accordance with MID / OIML R117 (example)

On devices for legal metrology, the hardware write protection must be activated after commissioning in many cases. This prevents a change in the parameterization of the devices.

To prevent deactivation of the hardware write protection or other manipulations during operation, the transmitter housing and the sensor housing connection box (with remote mount design) must be sealed.

For this purpose, a seal kit is available at ABB.

For the assembly of the seal, please observe the separate 'IN/FCX100/FCX400/MID/OIML-XA' instructions.

... Flowmeter sensor

Designs

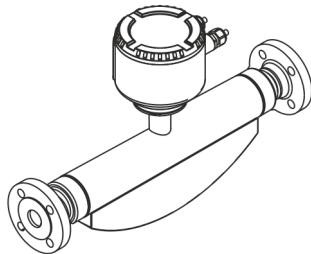


Figure 9: Sensor

Nominal diameter and measuring range

Nominal diameter	Q_{\max} in kg/h (lb/h)
DN 15 (½ in)	0 to 8,000 (0 to 17,637)
DN 25 (1 in)	0 to 35,000 (0 to 77,162)
DN 50 (2 in)	0 to 90,000 (0 to 198,416)
DN 80 (3 in)	0 to 250,000 (0 to 551,156)
DN 100 (4 in)	0 to 520,000 (0 to 1,146,404)
DN 150 (6 in)	0 to 860,000 (0 to 1,895,975)

Recommended flow range

Fluids:

- The recommended flow range is 5 to 100 % of Q_{\max} .
- Flow rates < 1 % of Q_{\max} should be avoided.

Gases:

- The flow velocity of gases in the meter tube should not up-scale 0.3 mach [approx. 100 m/s (328 ft/s)].
- Increased deviation in repeatability should be expected from a flow velocity of approx. 80 m/s (262 ft/s).
- The maximum flow range of gases depends on the operating density. Appropriate dimensioning guidelines are available at www.abb.com/flow.

Measuring accuracy

Reference conditions

Calibration fluid	Water
	<ul style="list-style-type: none"> Temperature: 25 °C (77 °F) ± 5 K Pressure: 2 to 4 bar (29 to 58 psi)
Ambient temperature	25 °C (77 °F) +10 K / -5 K
Power supply	Line voltage in accordance with name plate $U_N \pm 1\%$
Warm-up phase	30 min
Installation	<ul style="list-style-type: none"> Installation in accordance with Assembly Notes and Mounting positions No visible gas phase No external mechanical or hydraulic disturbances, particularly no cavitation
Output calibration	Pulse output

Measured error and repeatability

The measured error and repeatability are calculated as follows for the flow:

Scenario 1:

If

$$\text{Flow rate} \geq \frac{\text{Zero stability}}{(\text{base accuracy} / 100)}$$

Then:

- Maximum measured error:
± Base accuracy in % of measured value.
- Repeatability:
± $1/2 \times$ base accuracy in % of measured value.

Scenario 2:

If

$$\text{Flow rate} < \frac{\text{Zero stability}}{(\text{base accuracy} / 100)}$$

Then:

- Maximum measured error:
± ($\text{zero stability} / \text{measured value}$) × 100% of measured value.
- Repeatability:
± $1/2 \times (\text{zero point stability} / \text{measured value}) \times 100\%$ of measured value.

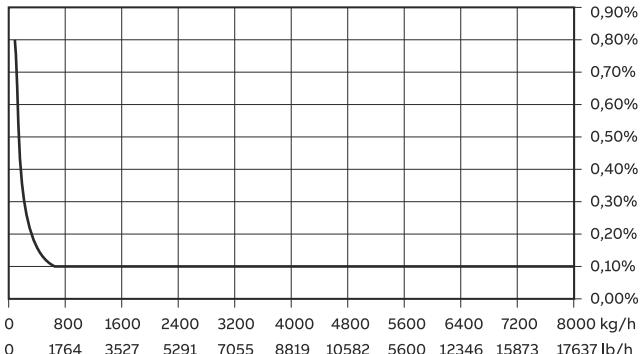


Figure 10: Measured error FCx150 DN 15 (example)

FCx150			
Measurem	Flow rate	Measured error*	Repeatability*
ent			
dynamic			
100:1	80 kg/h (176,4 lb/h)	≤ 0,8 %	0,4 %
50:1	160 kg/h (352,7 lb/h)	≤ 0,4 %	0,2 %
10:1	800 kg/h (1763,7 lb/h)	≤ 0,1 %	0,05 %
2:1	4000 kg/h (8818,5 lb/h)	≤ 0,1 %	0,05 %
1:1	8000 kg/h (17637 lb/h)	≤ 0,1 %	0,05 %

FCx150 – high accuracy			
Measurement	Flow rate	Measured error*	Repeatability*
dynamic			
100:1	80 kg/h (176,4 lb/h)	≤ 0,5 %	0,25 %
50:1	160 kg/h (352,7 lb/h)	≤ 0,25 %	0,122 %
10:1	800 kg/h (1763,7 lb/h)	≤ 0,1 %	0,05 %
2:1	4000 kg/h (8818,5 lb/h)	≤ 0,1 %	0,05 %
1:1	8000 kg/h (17637 lb/h)	≤ 0,1 %	0,05 %

* Enter measured error and repeatability as % of measured value

Measured error and base accuracy for liquids		
	FCx130	FCx150
Order code flow calibration	A, B, E, J, K, N	C, D, L, M
Order code density calibration	1	3, 4, 5
Mass flow*	± 0,4 % ± 0,25% ± 0,2%	± 0,15% ± 0,1% ± 0,2%
Volume flow*	± 0,4 % ± 0,25%	± 0,15% ± 0,11% ± 0,2%

Density	0,010 kg/l** 0,001 kg/l** 0,0004 kg/l**	0,002 kg/l** 0,001 kg/l** 0,0004 kg/l**
Repeatability for flow rate	Refer to page 15.	
Repeatability for density	0,002 kg/l** 0,001 kg/l** 0,0004 kg/l**	0,002 kg/l** 0,001 kg/l** 0,0004 kg/l**
Temperature	1K	

Measured error and base accuracy for gases		
	FCx130	FCx150
Order code flow calibration	A, B, E, J, K, N	C, D, L, M
Order code density calibration	1	3, 4, 5
Mass flow*	± 1%	± 0,5%
Temperature	1K	0,5 K

* Enter measured error and base accuracy as % of measured value

** For the density range from 0,5 to 1,8 kg/dm³

... Flowmeter sensor

... Measuring accuracy

Zero stability

Nominal diameter	FCx130	FCx150
Order code flow calibration	A, B, E, J, K, N	C, D, L, M
Order code density calibration	1	3, 4
DN 15 (½ in)	0.64 kg/h (1.41 lb/h)	
DN 25 (1 in)	2.16 kg/h (4.76 lb/h)	
DN 50 (2 in)	7.20 kg/h (15.87 lb/h)	
DN 80 (3 in)	20 kg/h (44 lb/h)	
DN 100 (4 in)	41.6 kg/h (91.7 lb/h)	
DN 150 (6 in)	68.8 kg/h (151.68 lb/h)	

Effect of the measuring medium temperature

	FCx130	FCx150
Order code flow calibration	A, B, E, J, K, N	C, D, L, M
Order code density calibration	1	3, 4
On flow rate	< ±0.005 % of Q_{\max} / 1 K	< ±0.0015 % of Q_{\max} / 1 K
On density	< 0.0001 kg/dm ³ per 1 K	

Effect of the operating pressure

Nominal diameter	Flow*	Density [kg/dm ³ / bar]
DN 15 (½ in)	-0.002 %	No effect
DN 25 (1 in)	-0.013 %	0.00035
DN 50 (2 in)	-0.010 %	0.00027
DN 80 (3 in)	-0.006 %	0.00019
DN 100 (4 in)	-0.009 %	0.00024
DN 150 (6 in)	-0.035 %	0.00045

* Influence of operating pressure as % of measured value per bar

Specifications

Pressure loss

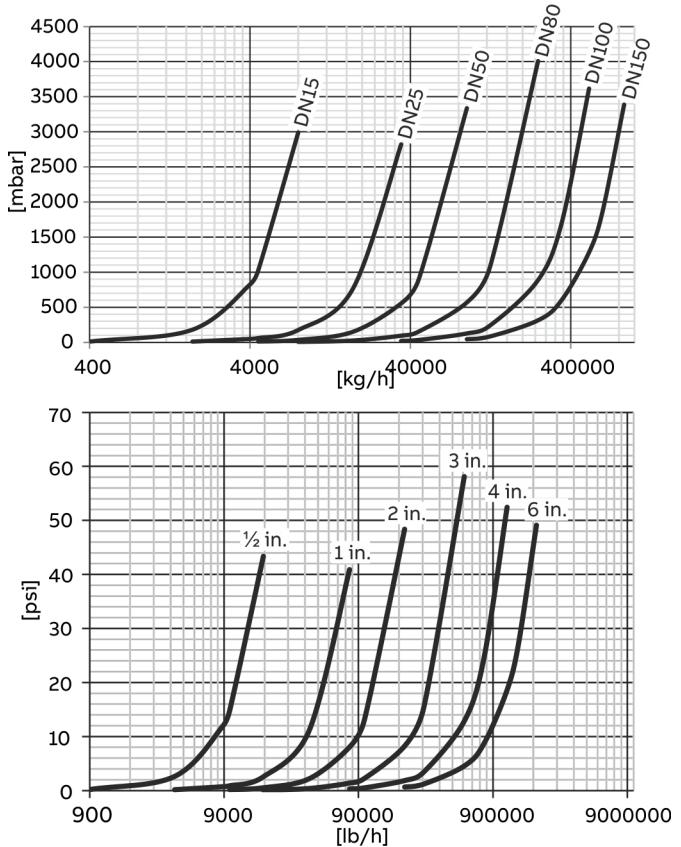


Figure 11: Pressure loss curve (measured with water, viscosity: 1 mPas)

Viscosity range

For dynamic viscosities ≥ 1 Pas (1000 mPas = 1000 cP), please consult ABB.

Temperature limits °C (°F)**Note**

When using the device in potentially explosive atmospheres, note the additional temperature data in **Temperature data** on page 48!

Measuring medium temperature T_{medium}

FCx130: -50 to 160 °C (-58 to 320 °F)

FCx150: -50 to 205 °C (-58 to 401 °F)

Ambient temperature $T_{\text{amb.}}$

-40 to 70 °C (-40 to 158 °F)

Note

In devices with order code '**Extended tower length – TE3**', from an ambient temperature of ≥ 65 °C (149 °F), the measuring medium temperature must be limited to a maximum of 140 °C (284 °F).

Process connections

For an overview of available process connection versions, see **Overview – models** on page 3.

Pressure ratings

The maximum permissible operating pressure is determined by the respective process connection, the temperature of the medium to be measured, the screws, and the gasket material. For an overview of available pressure ratings, see **Overview – models** on page 3.

Housing as a protective device (optional)**Order code PR5**

Maximum burst pressure 60 bar (870 psi)

Optional order code PR6 and PR7 on request

- Increased burst pressures up to 100 bar (1450 psi), possible for nominal diameters DN 15 to 100 (½ to 4 in.).
- Increased burst pressures up to 150 bar (2175 psi), possible for nominal diameters DN 15 to 80 (½ to 3 in.).
- Purge connections are available on request.

Pressure Equipment Directive

Conformity assessment in accordance with Category III, fluid group 1, gas. The pressure equipment is designed for load changes in accordance with the AD2000 specification sheet S1 Chapter 1.4 a) and b).

Note the corrosion resistance of the meter tube materials in relation to the measuring medium.

Installation lengths in accordance with NAMUR standards

The CoriolisMaster FCB100, FCH100 is the ideal device for use in accordance with NAMUR standards. While also conforming to other standards, the device can be ordered with installation lengths in accordance with NAMUR standards (order code '**Process connection – S5 / S7**'.

The exact installation lengths can be found in the tables in **Devices DN 15 to 150 in NAMUR standard installation lengths (order option S5, S7)** on page 33.

Materials for the transmitter terminal box**Housing**

- Aluminum EN AC-44200 (YL104)

or

- Stainless steel 1.4409 (ASTM CF3M)

Housing color (only for aluminum housing)

- RAL 9002

Layer thickness of the paint: 80 to 120 µm

... Flowmeter sensor

... Specifications

Materials for the sensor

Wetted components

Stainless steel

- 1.4404 (AISI 316L)

Stainless steel, polished

- 1.4404 (AISI 316L) or 1.4435 (AISI 316L) certified in accordance with EHEDG with sensor material (AISI 316L)

- C4 nickel alloy* (2.4610) or C22 nickel alloy* (2.4602)

Optional: Manufacture in accordance with NACE MR0175 and MR0103 (ISO 15156)

Sensor housing**

Stainless steel 1.4404 (AISI 316L), 1.4301 (AISI 304), 1.4308 (ASTM CF8)

* Hastelloy® C is a registered trademark of Haynes International. C4 and C22 nickel alloys are equivalent to Hastelloy® C4 and Hastelloy® C22.

** If the wetted parts of the sensor are made from nickel alloy then parts of the sensor housing (splitter) are also manufactured from nickel alloy. However, the prevailing parts remain manufactured from the specified material.

Roughness for flanges in accordance with EN 1092-1, ASME and JIS

	EN 1092-1 B1	EN 1092-1 B2
Pressure rating	≤ PN 40	≥ PN 63
Mean roughness value Ra	3.2 to 12.5 µm	0.8 to 3.2 µm
Roughness depth Rz	12.5 to 50.0 µm	3.2 to 12.5 µm

	ASME B 16.5	JIS B 2220	JIS 10K
Mean roughness value Ra	0.8 to 3.2 µm	3.2 to 6.3 µm	3.2 to 6.3 µm
Roughness depth Rz	3.2 to 12.5 µm	12.5 to 25 µm	12.5 to 25 µm

Material load for process connections

Note

You can reference the availability of the different process connections in the Online ABB Product Selection Assistant (PSA) for flow www.abb.com/flow-selector.

- Not all connections shown here are available in all the devices and designs.
- The permissible material load of the device can additionally differ from the material load of the connection. The permissible limit values (pressure rating / measuring medium temperature T_{medium}) can be found on the name plate.

Design	Nominal diameter	PS _{max}	TS _{max}	TS _{min}
Pipe fitting (DIN 11851)	DN 15 to DN 40 (½ to 1½ in)	40 bar (580 psi)	140 °C (284 °F)	-40 °C (-40 °F)
	DN 50 to DN 100 (2 to 4 in)	25 bar (363 psi)	140 °C (284 °F)	-40 °C (-40 °F)
	DN 125 to DN 200 (4 to 8 in)	16 bar (232 psi)	140 °C (284 °F)	-40 °C (-40 °F)
Pipe fitting (SMS 1145)	DN 25 to DN 80 (1 to 3 in)	6 bar (87 psi)	140 °C (284 °F)	-40 °C (-40 °F)
	DN 100 to DN 200 (3½ to 8 in)	10 bar (145 psi)	140 °C (284 °F)	-40 °C (-40 °F)
Tri-Clamp (DIN 32676)	DN 15 to DN 50 (½ to 2 in)	16 bar (232 psi)	140 °C (284 °F)	-40 °C (-40 °F)
	DN 65 to DN 100 (2½ to 4 in)	10 bar (145 psi)	140 °C (284 °F)	-40 °C (-40 °F)
	DN 125 to DN 200 (4 to 8 in)	16 bar (232 psi)	140 °C (284 °F)	-40 °C (-40 °F)
	DN 250 to DN 300 (10 to 12 in)	16 bar (232 psi)	140 °C (284 °F)	-40 °C (-40 °F)
	DN 350 to DN 400 (12½ to 16 in)	16 bar (232 psi)	140 °C (284 °F)	-40 °C (-40 °F)
ASME BPE Clamp	< DN 80 (< 3 in)	17,1 bar (248 psi)	121 °C (249,8 °F)	-40 °C (-40 °F)
	DN 80 (< 3 in)	15,5 bar (224,8 psi)	121 °C (249,8 °F)	-40 °C (-40 °F)
	DN 100 (< 4 in)	12,9 bar (187,1 psi)	121 °C (249,8 °F)	-40 °C (-40 °F)
	DN 125 (< 5 in)	12,9 bar (187,1 psi)	121 °C (249,8 °F)	-40 °C (-40 °F)
	DN 150 (< 6 in)	12,9 bar (187,1 psi)	121 °C (249,8 °F)	-40 °C (-40 °F)
NPT female thread	DN15 stainless steel 1.4404	179 bar (2596,2 psi)	150 °C (302 °F)	-40 °C (-40 °F)
	DN15 stainless steel 1.4404	163 bar (2364,1 psi)	205 °C (401 °F)	-40 °C (-40 °F)
	DN15 HC22 2.4602	267 bar (3872,5 psi)	150 °C (302 °F)	-40 °C (-40 °F)
	DN15 HC22 2.4602	243 bar (3524,4 psi)	205 °C (401 °F)	-40 °C (-40 °F)
	DN15 stainless steel 1.4404	243 bar (3524,4 psi)	205 °C (401 °F)	-40 °C (-40 °F)
	DN15 HC22 2.4602	243 bar (3524,4 psi)	205 °C (401 °F)	-40 °C (-40 °F)
	DN15 stainless steel 1.4404	243 bar (3524,4 psi)	205 °C (401 °F)	-40 °C (-40 °F)

Material load curves for flange devices

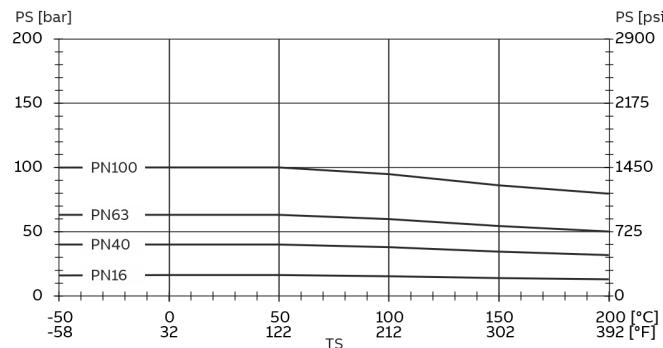


Figure 12: Stainless steel DIN flange 1.4404 (316L) up to DN 200 (8 in.)

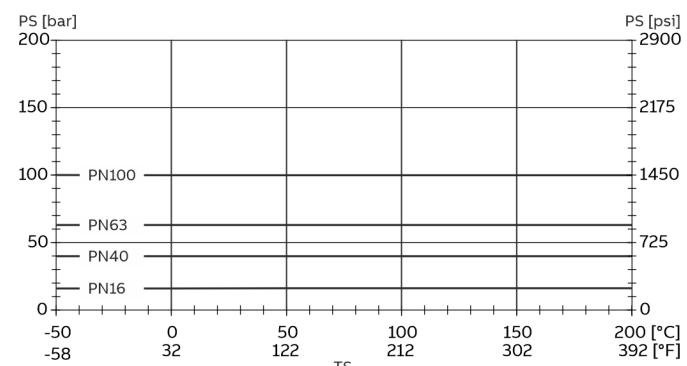


Figure 14: Nickel alloy DIN flange up to DN 200 (8 in.)

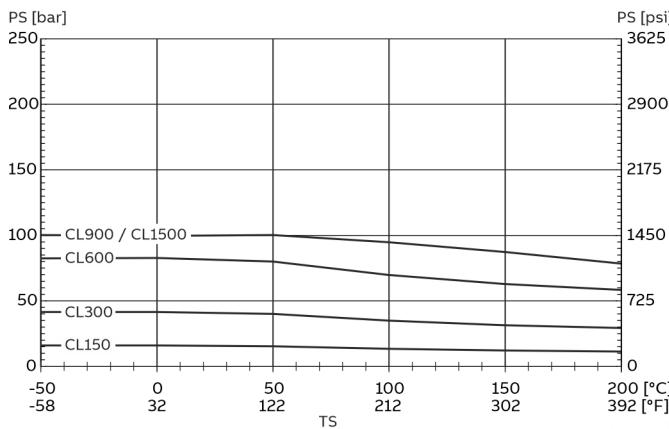


Figure 13: Stainless steel ASME flange 1.4404 (316L) up to DN 200 (8 in.)

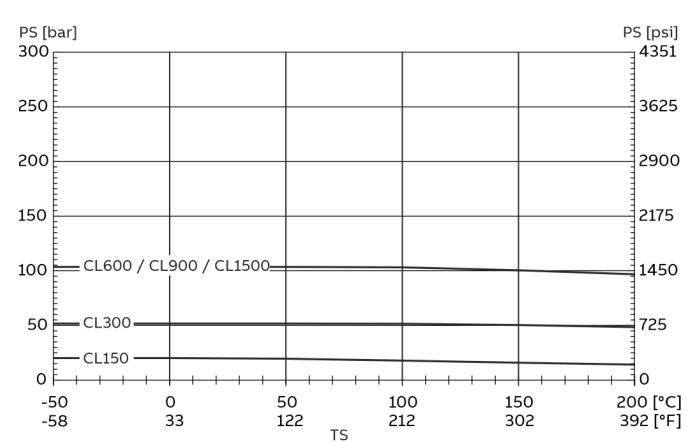


Figure 15: Nickel alloy ASME flange up to DN 200 (in.)


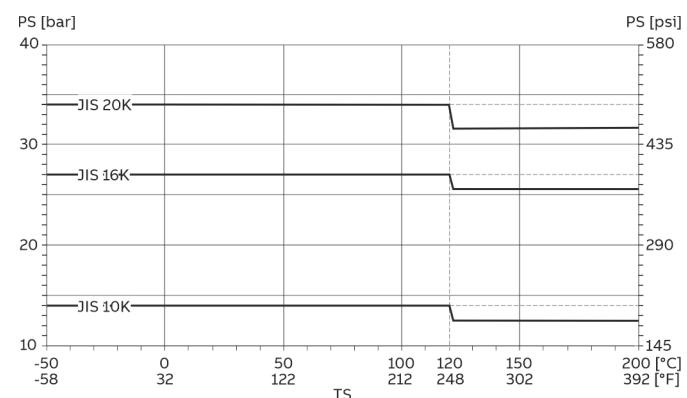


Figure 16: Stainless steel JIS B2220 flange 1.4435 or 1.4404 (AISI 316L) or nickel alloy

... Flowmeter sensor

Electrical connections

Models FCB130, FCB150, FCH130 and FCH150

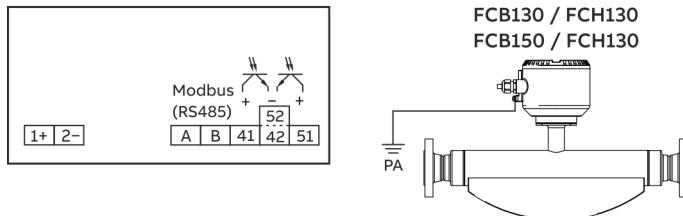

PA Potential equalization

Figure 17: Electrical connection

Connections for the power supply

DC voltage

Terminal	Function / comments
1+	+
2-	-

Connections for the outputs

Terminal	Function / comments
A / B	Modbus® RTU (RS485)
41 / 42	Passive digital output DO1 The output can be configured as a pulse output, frequency output or switch output.
51 / 52	Passive digital output DO2 The output can be configured as a pulse output or switch output.

Electrical data for inputs and outputs

Note

When using the device in potentially explosive atmospheres, note the additional connection data in **Use in potentially explosive atmospheres** on page 46!

Power supply

Supply voltage	11 to 30 V DC (ripple: ≤ 5 %)
Power consumption	S ≤ 5 VA

When connecting the devices, note the voltage drop on the cable. The operating voltage on the device must not be less than 11 V.


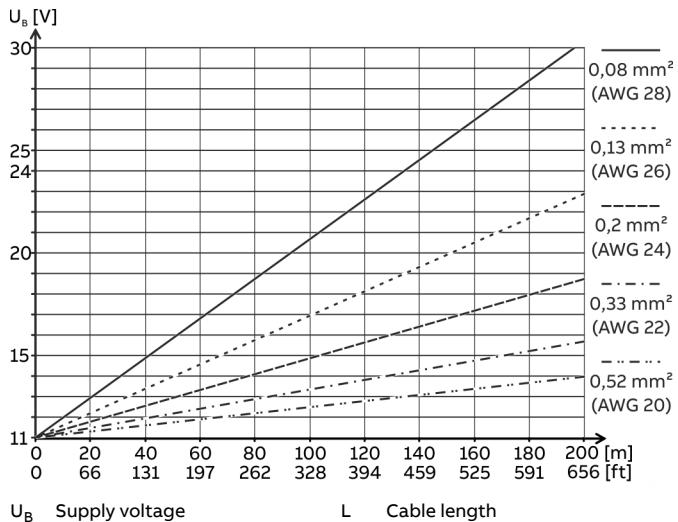


Figure 18: Maximum cable lengths (examples)

Digital output 41 / 42, 51 / 52

Can be configured via Modbus.

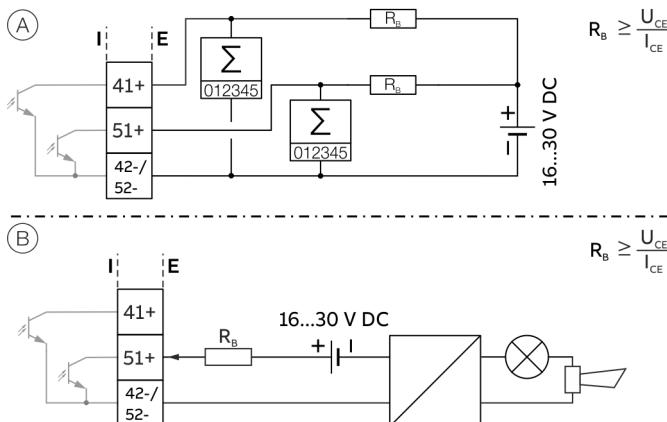

- (A) Passive digital output 41 / 42 as pulse or frequency output, Passive digital output 51 / 52 as pulse output
- (B) Passive digital output 51 / 52 as binary output

Figure 19: Passive digital outputs (I = internal, E = external)

Pulse / frequency output (passive)

Terminals	41 / 42 (pulse / frequency output) 51 / 52 (pulse output)
Output 'closed'	0 V ≤ U _{CEL} ≤ 3 V For f < 2.5 kHz: 2 mA < I _{CEL} < 30 mA For f > 2.5 kHz: 10 mA < I _{CEL} < 30 mA
Output 'open'	16 V ≤ U _{CER} ≤ 30 V DC 0 mA ≤ I _{CER} ≤ 0.2 mA
f _{max}	10.5 kHz
Pulse width	0.1 to 2000 ms

Binary output (passive)

Terminals	41 / 42, 51 / 52
Output 'closed'	0 V ≤ U _{CEL} ≤ 3 V 2 mA ≤ I _{CEL} ≤ 30 mA
Output 'open'	16 V ≤ U _{CER} ≤ 30 V DC 0 mA ≤ I _{CER} ≤ 0.2 mA
Switching function	Configurable

Note

- Digital output 51 / 52 **cannot** be configured as a frequency output.
- Terminals 42 / 52 have the same potential. Digital outputs 41 / 42 and 51 / 52 are not electrically isolated from each other.
- If you are using a mechanical counter, we recommend setting a pulse width of ≥ 30 ms and a maximum frequency of f_{max} ≤ 3 kHz.

Digital communication

Modbus® communication

Note

The Modbus® protocol is an unsecured protocol, as such the intended application should be assessed to ensure that these protocols are suitable before implementation.

Modbus is an open standard owned and administrated by an independent group of device manufacturers styled the Modbus Organization (www.modbus.org/).

Using the Modbus protocol allows devices made by different manufacturers to exchange information via the same communication bus, without the need for any special interface devices to be used.

Modbus protocol

Terminals	V1 / V2
Configuration	Via the Modbus interface or via the local operating interface in connection with a corresponding Device Type Manager (DTM)
Transmission	Modbus RTU - RS485 serial connection
Baud rate	2400, 4800, 9600, 19200, 38400, 56000, 57600, 115200 baud Factory setting: 9600 baud
Parity	None, even, odd Factory setting: odd
Stop bit	One, two Factory setting: One
IEEE format	Little endian, big endian Factory setting: Little endian
Typical response time	< 100 ms
Response delay time	0 to 200 milliseconds Factory setting: 10 milliseconds

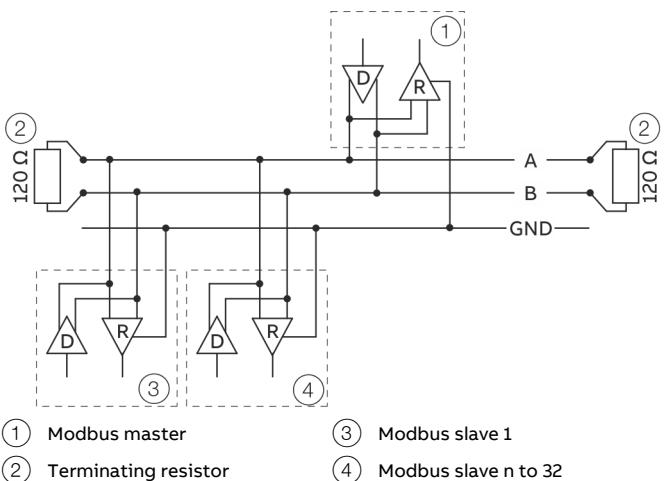


Figure 20: Communication with the Modbus protocol

Cable specification

The maximum permissible length is dependent on the baud rate, the cable (diameter, capacity and surge impedance), the number of loads in the device chain, and the network configuration (2-core or 4-core).

- At a baud rate of 9600 and with a conductor cross-section of at least 0.14 mm² (AWG 26), the maximum length is 1000 m (3280 ft).
- When using a 4-core cable as a 2-wire wiring system, the maximum length must be halved.
- The spur lines must be short, a maximum of 20 m (66 ft).
- When using a distributor with 'n' connections, each branch must have a maximum length of 40 m (131 ft) divided by 'n'.

The maximum cable length depends on the type of cable used. The following standard values apply:

- Up to 6 m (20 ft):
cable with standard shielding or twisted-pair cable.
- Up to 300 m (984 ft):
double twisted-pair cable with overall foil shielding and integrated earth cable.
- Up to 1200 m (3937 ft):
double twisted-pair cable with individual foil shielding and integrated earth cables. Example: Belden 9729 or equivalent cable.

A category 5 cable can be used for Modbus RS485 up to a maximum length of 600 m (1968 ft). For the symmetrical pairs in RS485 systems, a surge impedance of more than 100 Ω is preferred, especially at a baud rate of 19200 and above.

Dimensions

Meter tube inside diameter


Inside diameter of the meter tube of the Coriolis mass flowmeter CoriolisMaster FCB100, FCH100.

Nominal diameter	Meter tube inside diameter
DN 15 (½ in)	2 × 8 mm (2 × 0.31 in)
DN 25 (1 in)	2 × 16 mm (2 × 0.63 in)
DN 50 (2 in)	2 × 23.7 mm (2 × 0.93 in)
DN 80 (3 in)	2 × 36.62 mm (2 × 1.44 in)
DN 100 (4 in)	2 × 52.51 mm (2 × 2.07 in)
DN 150 (6 in)	2 × 68.9 mm (2 × 2.71 in)

Devices with meter tube nominal diameter DN 15 to 50 and flange DN 10 to 65

Sensor with wetted parts made from stainless steel.

All dimensions and weights are specified in mm (in) or kg (lb).

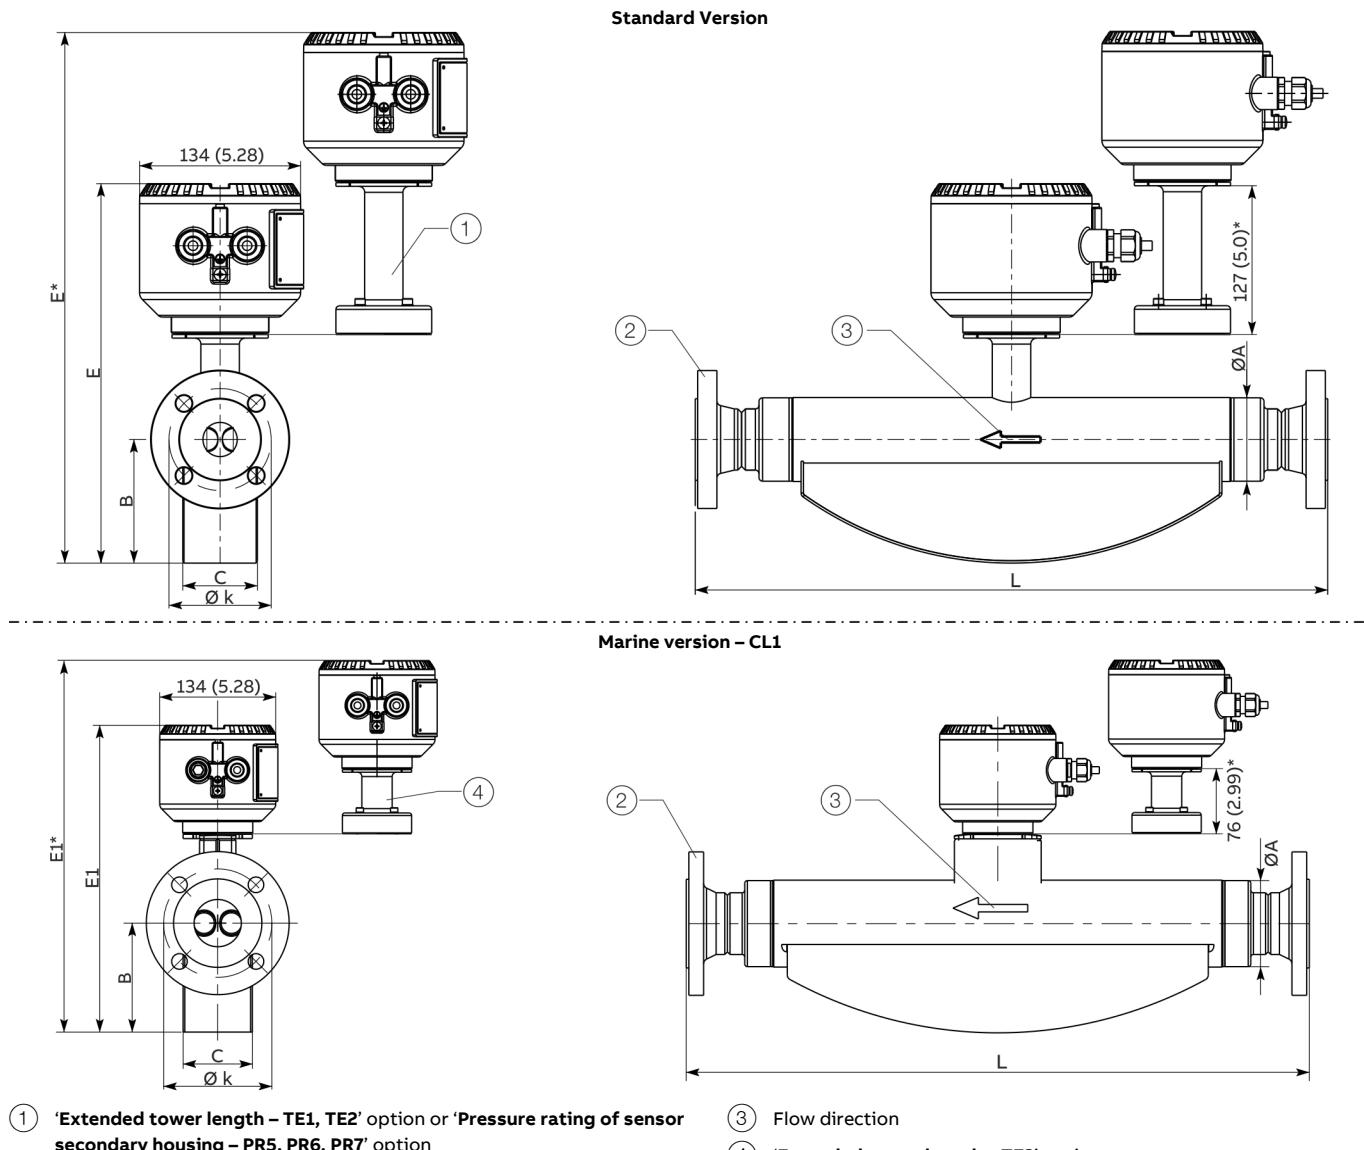

① 'Extended tower length – TE1, TE2' option or 'Pressure rating of sensor secondary housing – PR5, PR6, PR7' option

② Flange in accordance with EN 1092-1, ASME B16.5, ISO 7005
(connection dimensions for ASME flanges in accordance with ASME B16.5 (ANSI))

③ Flow direction

④ 'Extended tower length – TE3' option

* Standard version: devices with 'Extended tower length – TE1, TE2' option or 'Pressure rating of sensor secondary housing' option

** Marine version – CL1: devices with 'Extended tower length – TE3' option

Figure 1: Remote mount design

... Flowmeter sensor

... Dimensions

Meter tube nominal diameter DN 15 (½ in)

DN / process connection		L	Ø k	Ø A	B	C	E	E1	Weight max.
10 (¾ in)	PN 40 (EN 1092-1 B1)	385 (15.2)	60 (2.4)	44.5 (1.8)	80 (3.2)	49 (1.93)	283 (11.1) 410*	(16.1*) 357** (14.1**)	13 (28.7)
	JIS 10K	385 (15.2)	65 (2.6)						
	JIS 16K	385 (15.2)	65 (2.6)						
	JIS 20K	385 (15.2)	65 (2.6)						
15 (½ in)	PN 40 (EN 1092-1 B1)	385 (15.2)	65 (2.6)						
	PN 63 (EN 1092-1 B2)	403 (15.9)	75 (3.0)						
	PN 100 (EN 1092-1 B2)								
	CL150 (ASME B16.5)	435 (17.1)	60.5 (2.4)						
	CL300 (ASME B16.5)	421 (16.6)	66.5 (2.6)						
	CL600 (ASME B16.5)								
	CL900 (ASME B16.5)	421 (16.6)	82.6 (3.3)						
20 (¾ in)	CL1500 (ASME B16.5)								
	JIS 10K	385 (15.2)	70 (2.8)						
	JIS 16K	385 (15.2)	70 (2.8)						
	JIS 20K	385 (15.2)	70 (2.8)						
	PN 40 (EN 1092-1 B1)	421 (16.6)	75 (3.0)						
	CL150 (ASME B16.5)	421 (16.6)	69.9 (2.8)						
	JIS 10K	421 (16.6)	75 (3.0)						
25 (1 in)	JIS 16K	421 (16.6)	75 (3.0)						
	JIS 20K	421 (16.6)	75 (3.0)						

Meter tube nominal diameter DN 25 (1 in)

DN / process connection		L	Ø k	Ø A	B	C	E	E1	Weight max.
20 (¾ in)	PN 40 (EN 1092-1 B1)	576 (22.7)	75 (3.0)	69.5 (2.74)	103 (4.06)	62 (2.44)	324 (12.8)	324 (12.8)	15 (33.1)
	CL150 (ASME B16.5)	575 (22.6)	69.9 (2.8)				451* (17.8*)	398** (15.7**)	
	JIS 10K	576 (22.7)	75 (3.0)						
	JIS 16K	576 (22.7)	75 (3.0)						
	JIS 20K	576 (22.7)	75 (3.0)						
25 (1 in)	PN 40 (EN 1092-1 B1)	525 (20.7)	85 (3.3)						
	PN 63 (EN 1092-1 B2)	564 (22.2)	100 (3.9)						
	PN 100 (EN 1092-1 B2)								
	CL150 (ASME B16.5)	575 (22.6)	79.2 (3.1)						
	CL300 (ASME B16.5)	576 (22.7)	88.9 (3.5)						
	CL600 (ASME B16.5)								
	CL900 (ASME B16.5)	576 (22.7)	101.6 (4.0)						
	CL1500 (ASME B16.5)								
	JIS 10K	525 (20.7)	90 (3.54)						
	JIS 16K	525 (20.7)	90 (3.54)						
	JIS 20K	525 (20.7)	90 (3.54)						
40 (1½ in)	PN 40 (EN 1092-1 B1)	576 (22.7)	110 (4.33)						
	PN 63 (EN 1092-1 B2)	572 (22.5)	125 (4.92)						
	PN 100 (EN 1092-1 B2)								
	CL150 (ASME B16.5)	576 (22.7)	98.6 (3.88)						
	CL300 (ASME B16.5)	576 (22.7)	114.3 (45.0)						
	CL600 (ASME B16.5)								
	JIS 10K	576 (22.7)	105 (4.13)						
	JIS 16K	576 (22.7)	105 (4.13)						
	JIS 20K	576 (22.7)	105 (4.13)						

* Standard version: devices with '**Extended tower length – TE1, TE2**' option or '**Pressure rating of sensor secondary housing**' option

** Marine version – CL1: devices with '**Extended tower length – TE3**' option

Tolerance for dimension L: +0 / -3 mm (+0 / -0.118 in)

... Flowmeter sensor

... Dimensions

Meter tube nominal diameter DN 50 (2 in)

DN / process connection		L	Ø k	Ø A	B	C	E	E1	Weight max.
40 (1½ in)	PN 40 (EN 1092-1 B1)	763 (30)	110 (4.33)	99 (3.9)	126 (4.96)	80 (3.15)	354 (13.9)	354 (13.9)	31 (68.3)
	PN 63 (EN 1092-1 B2)	745 (29.33)	125 (4.92)				481* (18.94*)	428** (16.9**)	
	PN 100 (EN 1092-1 B2)								
	CL150 (ASME B16.5)	763 (30)	98.6 (3.88)						
	CL300 (ASME B16.5)	756 (29.76)	114.3 (4.5)						
	CL600 (ASME B16.5)								
	CL900 (ASME B16.5)	780 (30.71)	124 (4.88)						
	CL1500 (ASME B16.5)								
	JIS 10K	763 (30)	105 (4.13)						
	JIS 16K	763 (30)	105 (4.13)						
	JIS 20K	763 (30)	105 (4.13)						
50 (2 in)	PN 40 (EN 1092-1 B1)	715 (28.15)	125 (4.92)						
	PN 63 (EN 1092-1 B2)	745 (29.3)	135 (5.31)						
	PN 100 (EN 1092-1 B2)	745 (29.33)	145 (5.71)						
	CL150 (ASME B16.5)	715 (28.15)	120.7 (4.75)						
	CL300 (ASME B16.5)	763 (30)	127 (5.0)						
	CL600 (ASME B16.5)	773 (30.43)	127 (5.0)						
	CL900 (ASME B16.5)	790 (31.1)	165.1 (6.5)						
	CL1500 (ASME B16.5)								
	JIS 10K	715 (28.15)	120 (4.72)						
	JIS 16K	715 (28.15)	120 (4.72)						
	JIS 20K	715 (28.15)	120 (4.72)						
65 (2½ in)	PN 40 (EN 1092-1 B1)	763 (30)	145 (5.71)						
	CL150 (ASME B16.5)	756 (29.76)	139.7 (5.5)						
	CL900 (ASME B16.5)	800 (31.5)	190.5 (7.5)						
	CL1500 (ASME B16.5)								
	JIS 10K	763 (30)	140 (5.51)						
	JIS 16K	763 (30)	140 (5.51)						
	JIS 20K	763 (30)	140 (5.51)						

* Standard version: devices with 'Extended tower length – TE1, TE2' option or 'Pressure rating of sensor secondary housing' option


** Marine version – CL1: devices with 'Extended tower length – TE3' option

Tolerance for dimension L: +0 / -3 mm (+0 / -0.118 in)

Devices with meter tube nominal diameter DN 80 and flange DN 65 to 100

Sensor with wetted parts made from stainless steel.

All dimensions and weights are specified in mm (in) or kg (lb).

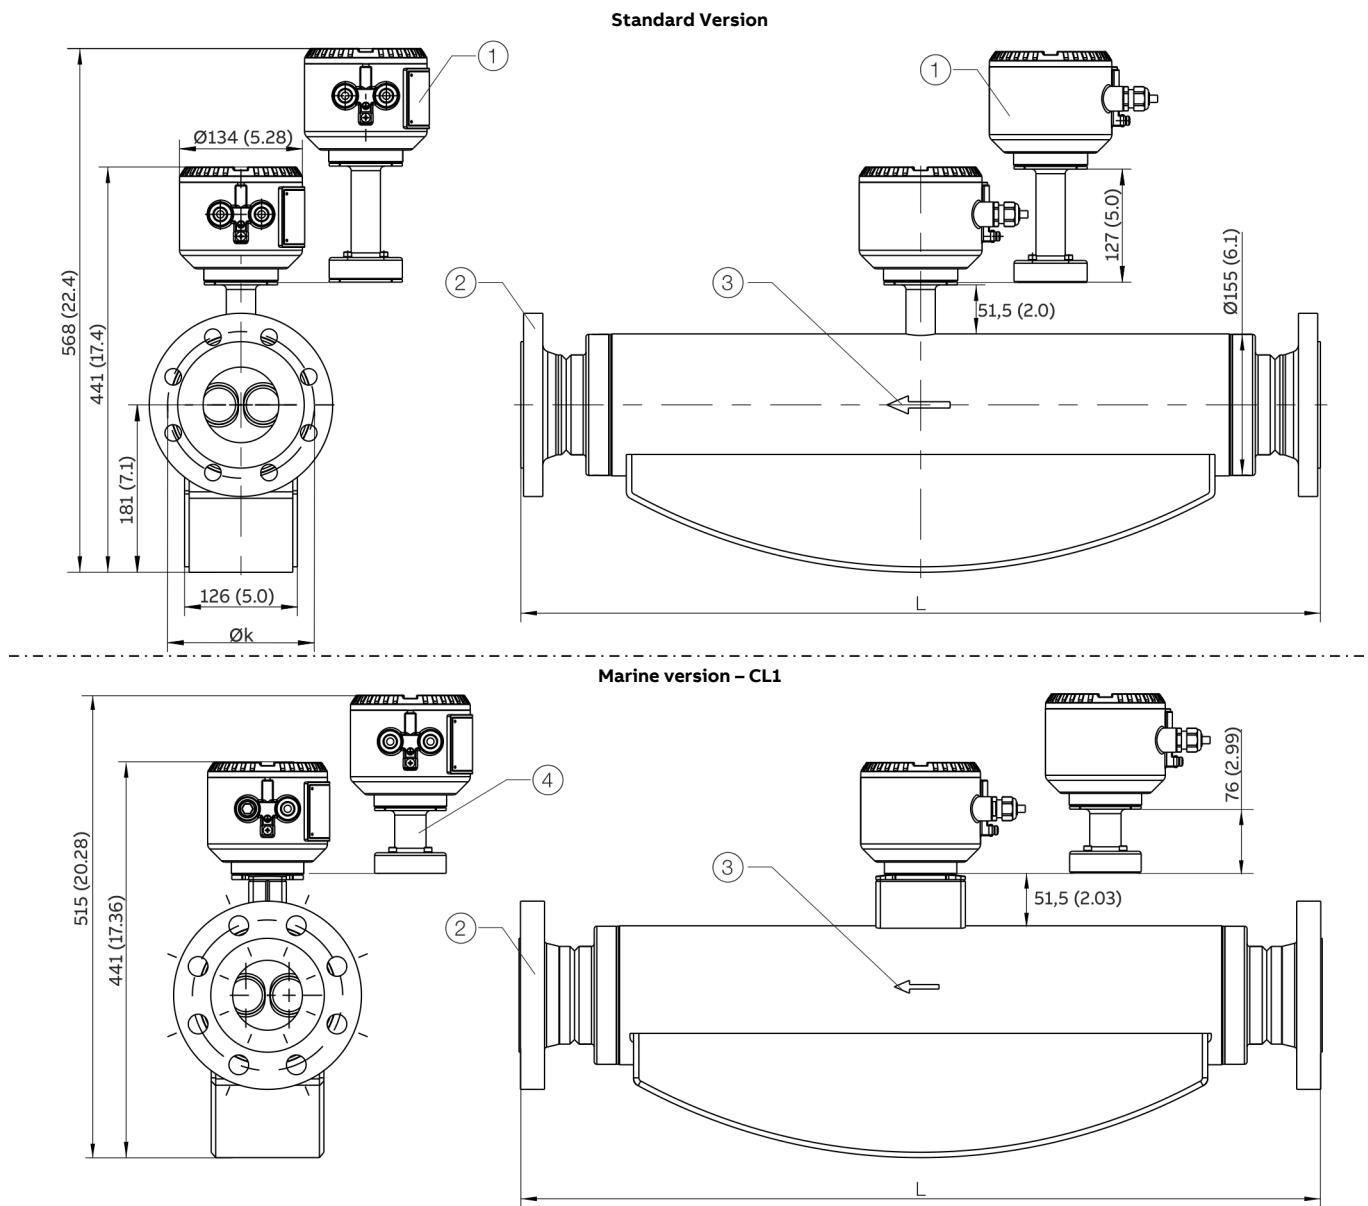

- (1) 'Extended tower length – TE1, TE2' option or 'Pressure rating of sensor secondary housing – PR5, PR6, PR7' option

- (2) Flange in accordance with EN 1092-1, ASME B16.5, ISO 7005
(connection dimensions for ASME flanges in accordance with ASME B16.5 (ANSI))

- (3) Flow direction

- (4) 'Extended tower length – TE3' option

Figure 2: Remote mount design

... Flowmeter sensor

... Dimensions

Meter tube nominal diameter DN 80 (3 in)				
DN / process connection		L	Ø k	Weight max.
65 (2½ in)	PN 16 (EN 1092-1 B1)	—*	—*	—*
	PN 40 (EN 1092-1 B1)	910 (35.83)	145 (5.71)	74 (163.1)
	PN 63 (EN 1092-1 B2)		160 (6.3)	78 (172.0)
	PN 100 (EN 1092-1 B2)		170 (6.69)	82 (180.8)
	CL150 (ASME B16.5)	920 (36.22)	123 (4.48)	74 (163.1)
	CL300 (ASME B16.5)	920 (36.22)	149.4 (5.88)	76 (167.6)
	CL600 (ASME B16.5)			77 (169.8)
	CL900 (ASME B16.5)	965 (37.99)	190.5 (7.5)	94 (207.2)
	CL1500 (ASME B16.5)			
	JIS 10K	910 (35.83)	140 (5.5)	74 (163.1)
80 (3 in)	JIS 16K	910 (35.83)	140 (5.5)	74 (163.1)
	JIS 20K	920 (36.22)	140 (5.5)	74 (163.1)
	PN 16 (EN 1092-1 B1)	870 (34.25)	160 (6.30)	74 (163.1)
	PN 40 (EN 1092-1 B1)			75 (165.4)
	PN 63 (EN 1092-1 B2)	910 (35.83)	170 (6.69)	79 (174.2)
	PN 100 (EN 1092-1 B2)		180 (7.09)	85 (187.4)
	CL150 (ASME B16.5)	880 (34.65)	152.4 (6.00)	76 (165.4)
	CL300 (ASME B16.5)	895 (35.24)	168.1 (6.62)	79 (174.2)
	CL600 (ASME B16.5)	920 (36.22)		82 (180.8)
	CL900 (ASME B16.5)	1100 (43.31)	190.5 (7.50)	94 (207.2)
100 (4 in)	CL1500 (ASME B16.5)	1300 (51.18)	203.2 (8.00)	106 (233.7)
	JIS 10K	870 (34.25)	150 (5.91)	75 (165.4)
	JIS 16K	870 (34.25)	150 (5.91)	75 (165.4)
	JIS 20K	910 (35.83)	150 (5.91)	75 (165.4)
	PN 16 (EN 1092-1 B1)	875 (34.45)	180 (7.09)	75 (165.4)
	PN 40 (EN 1092-1 B1)		190 (7.48)	76 (167.5)
	PN 63 (EN 1092-1 B2)	1060 (41.73)	200 (7.87)	86 (189.6)
	PN 100 (EN 1092-1 B2)	1080 (42.52)	210 (8.27)	94 (207.2)
	CL150 (ASME B16.5)	880 (34.65)	190.5 (7.50)	77 (169.8)
	CL300 (ASME B16.5)	1075 (42.32)	200.2 (7.88)	91 (200.6)
	CL600 (ASME B16.5)	1100 (43.31)	215.9 (8.50)	101 (222.7)
	CL900 (ASME B16.5)	1130 (44.49)	234.9 (9.25)	111 (244.7)
	CL1500 (ASME B16.5)	1150 (45.28)	241.3 (9.50)	126 (277.8)
	JIS 10K	1060 (41.7)	175 (6.9)	86 (189.6)
	JIS 16K	1060 (41.7)	175 (6.9)	85 (187.4)
	JIS 20K	1060 (41.7)	175 (6.9)	85 (187.4)


* On request

Tolerance for dimension L: +0 / -3 mm (+0 / -0.118 in)

Devices with meter tube nominal diameter DN 100 and flange DN 80 to 150

Sensor with wetted parts made from stainless steel.

All dimensions and weights are specified in mm (in) or kg (lb).

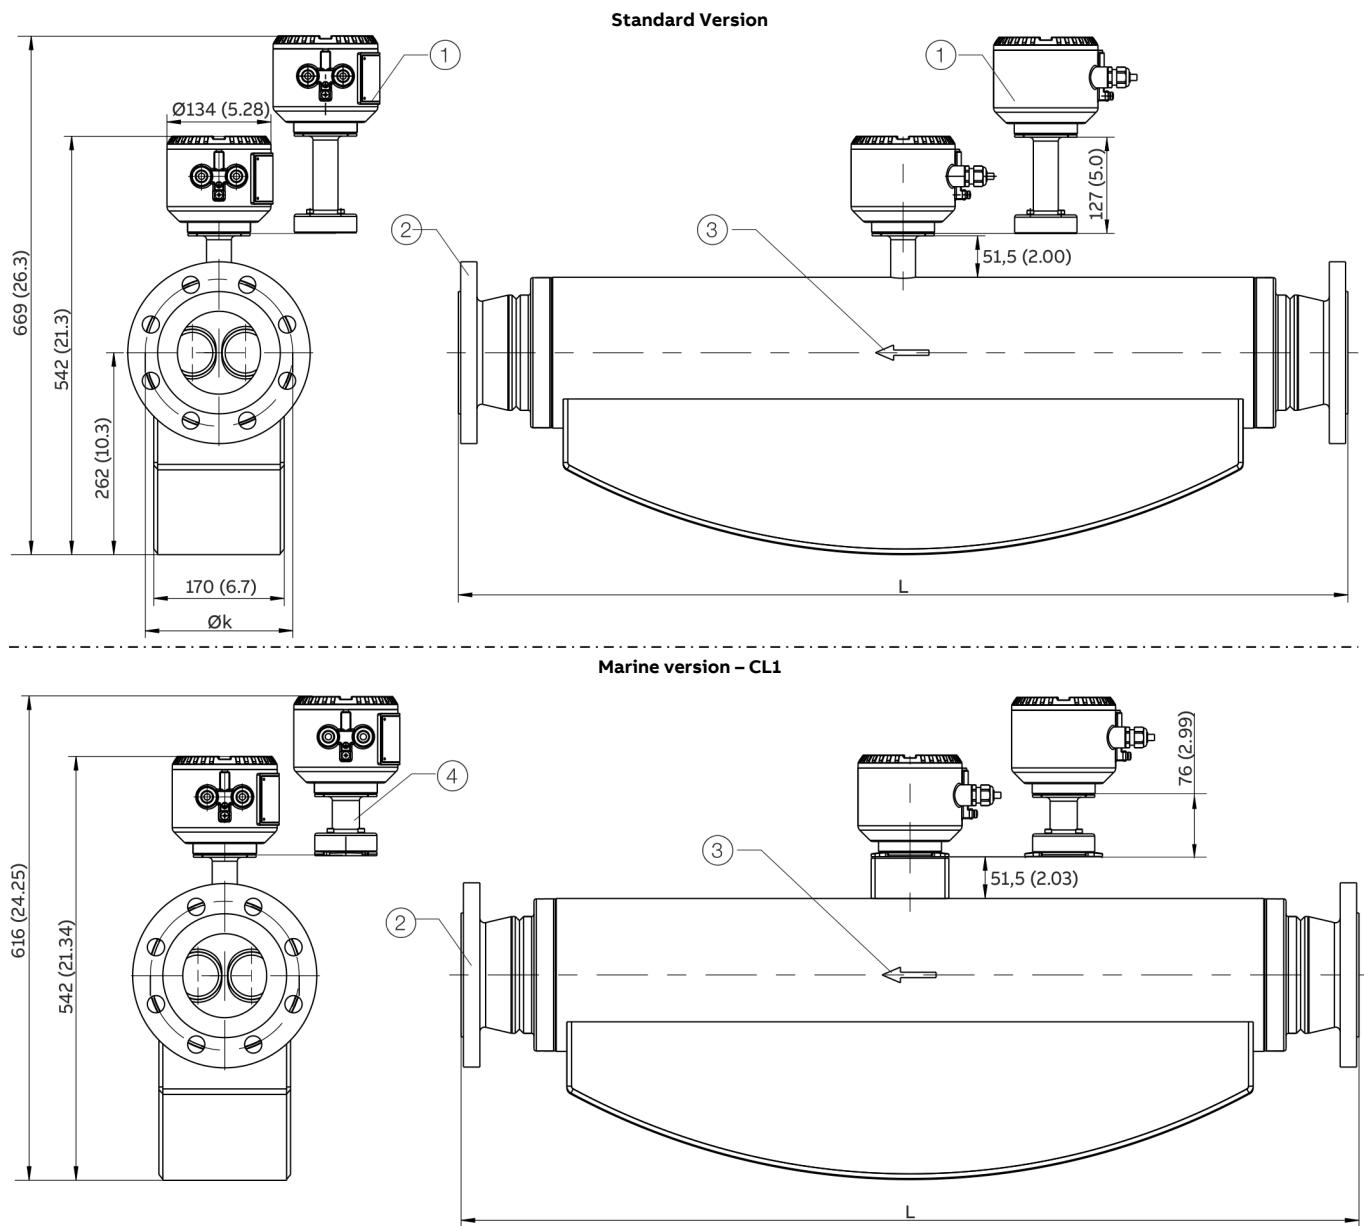

- (1) 'Extended tower length – TE1, TE2' option or 'Pressure rating of sensor secondary housing – PR5, PR6, PR7' option
- (2) Flange in accordance with EN 1092-1, ASME B16.5, ISO 7005
(connection dimensions for ASME flanges in accordance with ASME B16.5 (ANSI))

- (3) Flow direction
- (4) 'Extended tower length – TE3' option

Figure 3: Remote mount design

... Flowmeter sensor

... Dimensions

Meter tube nominal diameter DN 100 (4 in)

DN / process connection	L	Ø k	Weight max.
80 (3 in)	PN 16 (EN 1092-1 B1)	1222 (48.11) ¹⁾	160 (6.30)
	PN 40 (EN 1092-1 B1)		126 (278)
	PN 63 (EN 1092-1 B2)	1234 (48.58) ¹⁾	170 (6.69)
	PN 100 (EN 1092-1 B2)		180 (7.09)
	CL150 (ASME B16.5)	1244 (48.98) ¹⁾	152.4 (6.00)
	CL300 (ASME B16.5)		168.1 (6.62)
	CL600 (ASME B16.5)		168.1 (6.62)
	CL900 (ASME B16.5)	1470 (57.87) ¹⁾	190.5 (7.50)
	CL1500 (ASME B16.5)	1500 (59.05) ¹⁾	203.2 (8.00)
	JIS 10K	1275 (50.20) ¹⁾	150 (5.91)
100 (4 in)	JIS 16K	1275 (50.20) ¹⁾	150 (5.91)
	JIS 20K	1275 (50.20) ¹⁾	150 (5.91)
	PN 16 (EN 1092-1 B1)	1123 (44.21) ²⁾	180 (7.09)
	PN 40 (EN 1092-1 B1)	1146 (45.12) ²⁾	190 (7.48)
	PN 63 (EN 1092-1 B2)	1304 (51.34) ¹⁾	138 (5.43)
	PN 100 (EN 1092-1 B2)	1334 (52.52) ¹⁾	150 (5.91)
	CL150 (ASME B16.5)	1145 (45.08) ²⁾	190.5 (7.50)
	CL300 (ASME B16.5)	1320 (51.97) ²⁾	200.2 (7.88)
	CL600 (ASME B16.5)	1336 (52.60) ³⁾	215.9 (8.50)
	CL900 (ASME B16.5)	1380 (54.33) ¹⁾	234.9 (9.25)
150 (6 in)	CL1500 (ASME B16.5)	1400 (55.12) ¹⁾	241.3 (9.50)
	JIS 10K	1150 (45.28) ¹⁾	175 (6.89)
	JIS 16K	1150 (45.28) ¹⁾	175 (6.89)
	JIS 20K	1150 (45.28) ¹⁾	175 (6.89)
	PN 16 (EN 1092-1 B1)	1255 (49.41) ²⁾	240 (9.44)
	PN 40 (EN 1092-1 B1)	1297 (51.06) ¹⁾	250 (9.84)
	CL150 (ASME B16.5)	1252 (49.29) ³⁾	241.3 (9.50)
	CL600 (ASME B16.5)	1400 (55.12) ¹⁾	-
	JIS 10K	1300 (51.18) ¹⁾	240 (9.44)
	JIS 16K	1300 (51.18) ¹⁾	240 (9.44)
	JIS 20K	1308 (51.50) ¹⁾	240 (9.44)

L dimension tolerances

1) +0 / -15 mm (+0 / -0.59 in)

2) +0 / -5 mm (+0 / -0.20 in)

3) +0 / -8 mm (+0 / -0.31 in)

Devices with meter tube nominal diameter DN 150 and flange DN 100 to DN 200

Sensor with wetted parts made from stainless steel.

All dimensions and weights are specified in mm (in) or kg (lb).

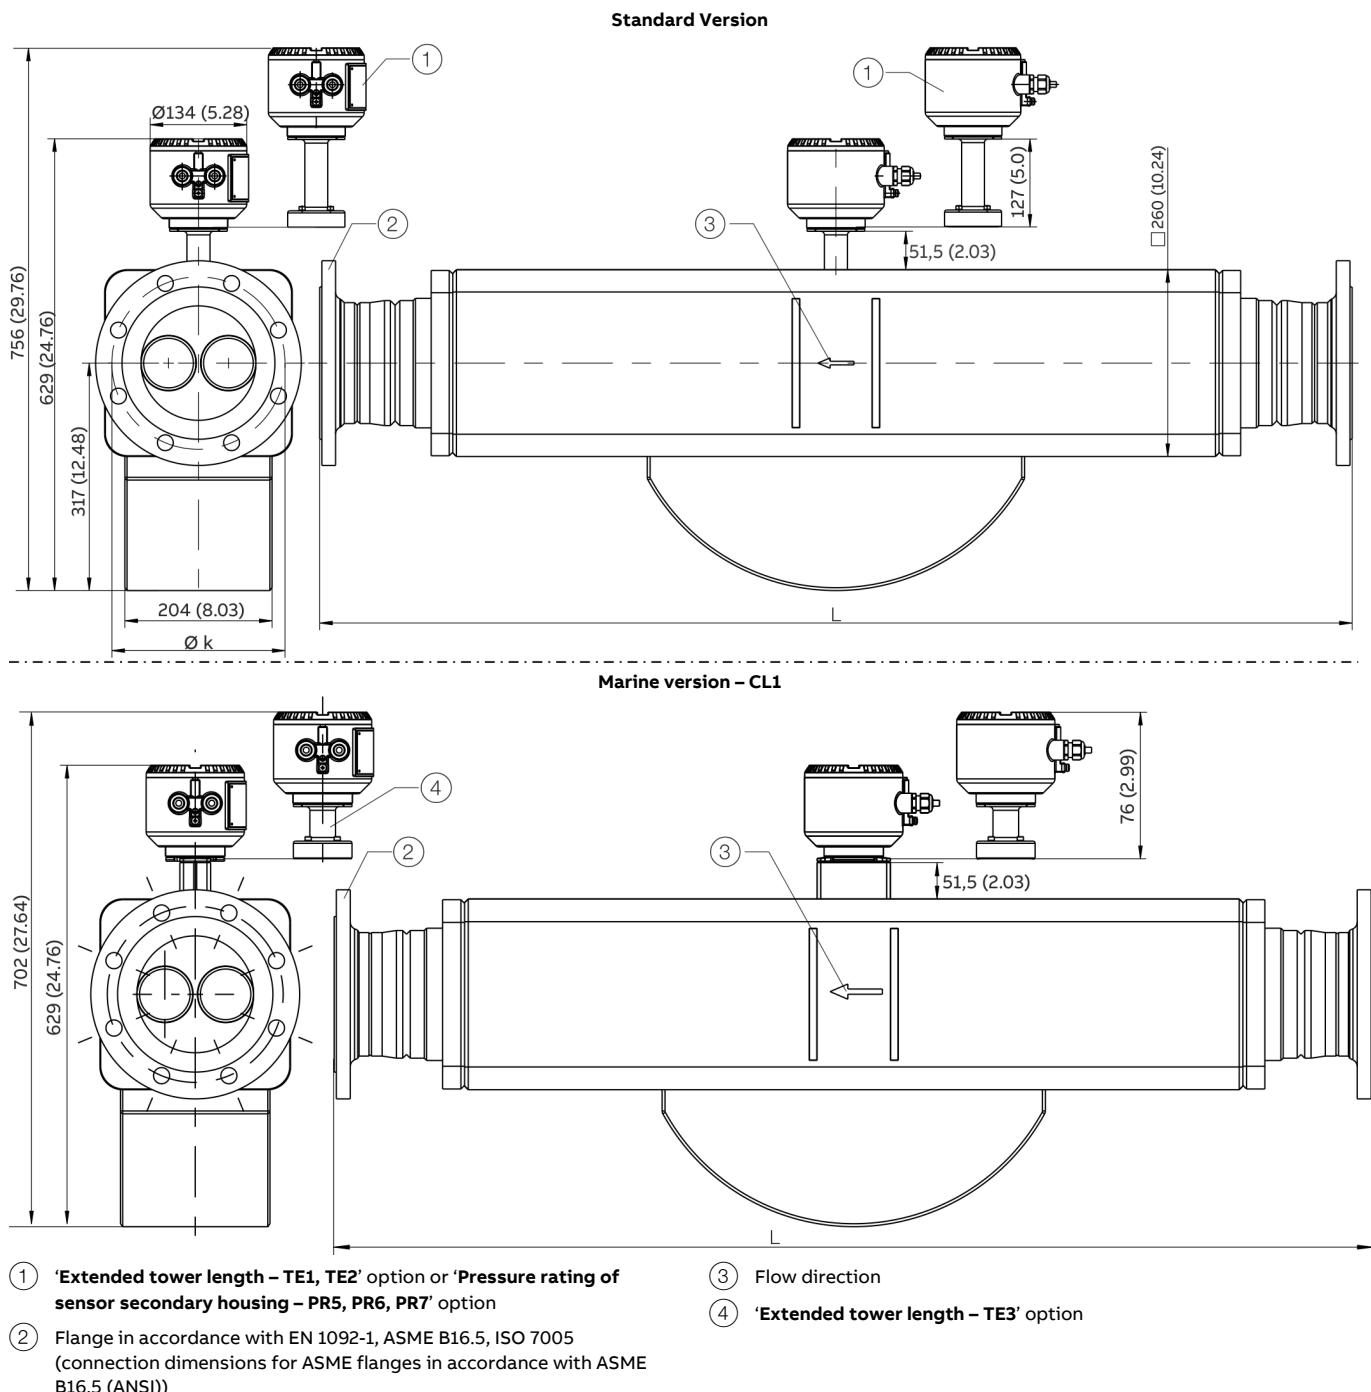


Figure 4: Remote mount design

... Flowmeter sensor

... Dimensions

Meter tube nominal diameter DN 150 (6 in)

DN / process connection	L	Ø k	Weight max.
100 (4 in)	PN 16 (EN 1092-1 B1)	1569 (61.77) ¹⁾	175 (386)
	PN 40 (EN 1092-1 B1)	1599 (62.95) ¹⁾	179 (395)
	CL150 (ASME B16.5)	1630 (64.17) ¹⁾	182 (401)
	CL300 (ASME B16.5)	1650 (64.96) ¹⁾	188 (414)
	CL600 (ASME B16.5)	1675 (65.94) ¹⁾	198 (437)
	CL900 (ASME B16.5)	1705 (67.13) ¹⁾	208 (459)
	CL1500 (ASME B16.5)	1725 (67.91) ¹⁾	223 (492)
	JIS 10K	1485 (58.46) ¹⁾	179 (395)
	JIS 16K	1485 (58.46) ¹⁾	181 (399)
	JIS 20K	1485 (58.46) ¹⁾	181 (399)
150 (6 in)	PN 16 (EN 1092-1 B1)	1421 (55.94) ¹⁾	178 (392)
	PN 40 (EN 1092-1 B1)	1459 (57.44) ²⁾	186 (410)
	CL150 (ASME B16.5)	1482 (58.35) ³⁾	185 (408)
	CL300 (ASME B16.5)	1503 (59.17) ³⁾	203 (448)
	CL600 (ASME B16.5)	1555 (61.22) ¹⁾	225 (496)
	CL900 (ASME B16.5)	1605 (63.19) ¹⁾	249 (549)
	CL1500 (ASME B16.5)	1665 (65.55) ¹⁾	291 (642)
	JIS 10K	1425 (56.10) ¹⁾	186 (410)
	JIS 16K	1456 (57.32) ¹⁾	187 (412)
	JIS 20K	1464 (57.64) ¹⁾	187 (412)
200 (8 in)	PN 16 (EN 1092-1 B1)	-*	-*
	PN 40 (EN 1092-1 B1)	1637 (64.45) ¹⁾	209 (461)
	CL150 (ASME B16.5)	1650 (64.96) ¹⁾	204 (450)
	CL300 (ASME B16.5)	1664 (65.51) ³⁾	229 (505)
	CL600 (ASME B16.5)	1730 (68.11) ¹⁾	-
	JIS 10K	1583 (62.32) ¹⁾	209 (461)
	JIS 16K	1615 (63.58) ¹⁾	210 (463)
	JIS 20K	1623 (63.90) ¹⁾	210 (463)

* On request


L dimension tolerances

- 1) +0 / -20 mm (+0 / -0.79 in)
- 2) +0 / -5 mm (+0 / -0.20 in)
- 3) +0 / -8 mm (+0 / -0.31 in)

Devices DN 15 to 150 in NAMUR standard installation lengths (order option S5, S7)

Sensor with wetted parts made from stainless steel.

All dimensions and weights are specified in mm (in) or kg (lb).

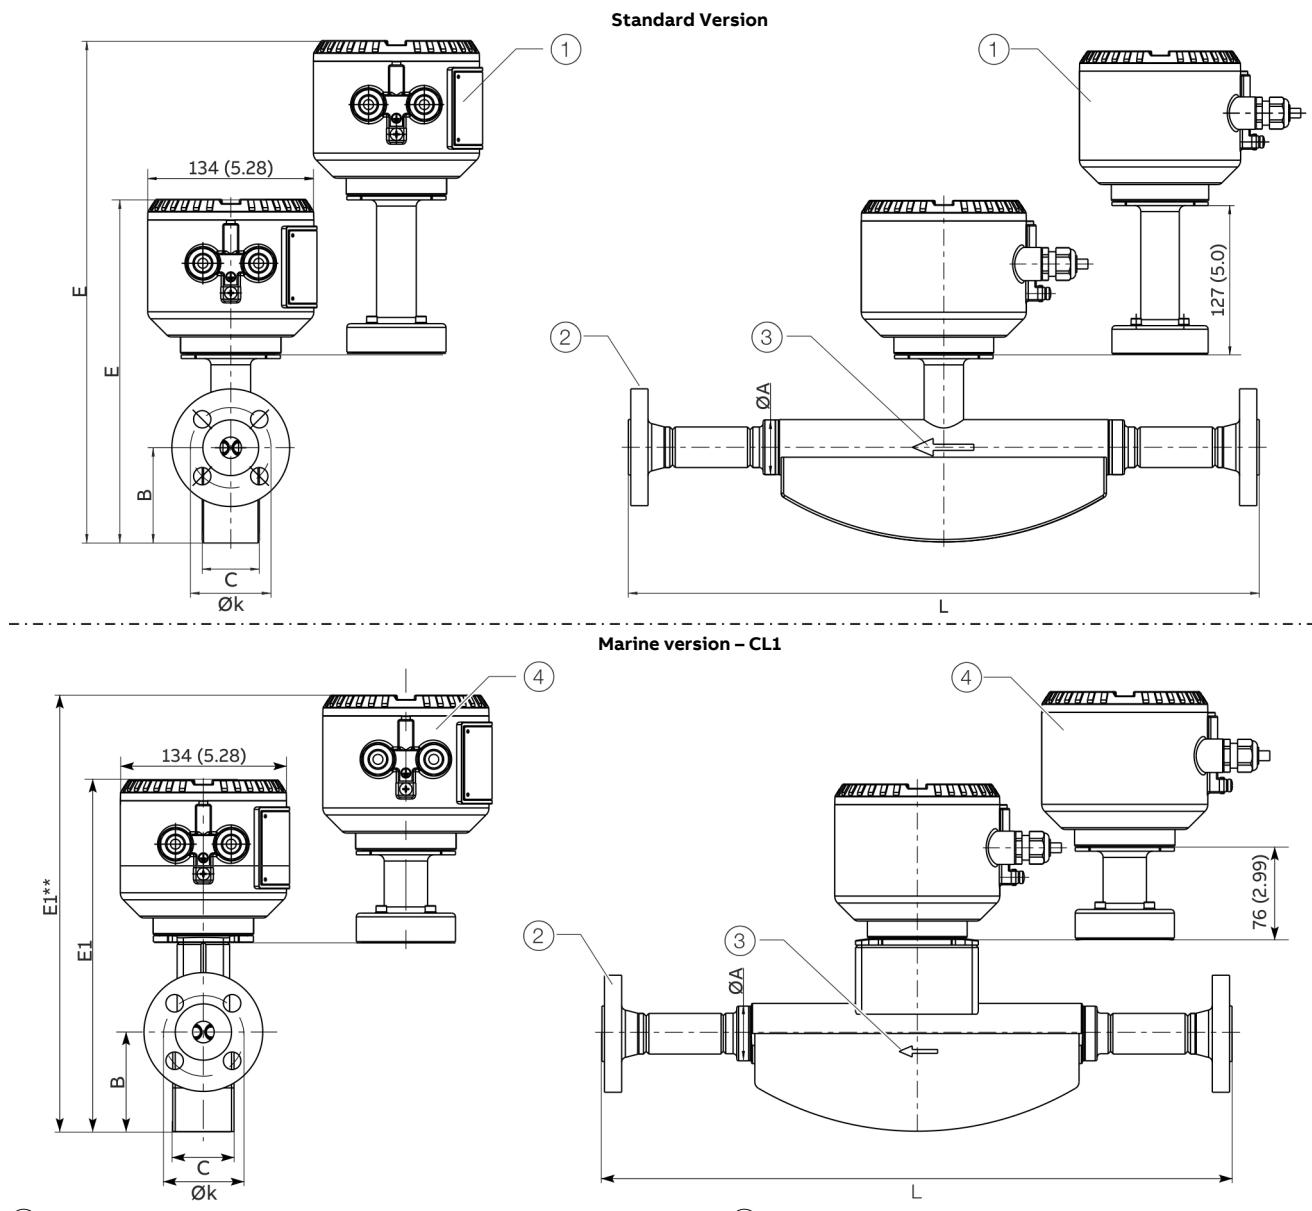

* Standard design: Devices with 'Extended tower length – TE1, TE2' option or 'Pressure rating of sensor secondary housing – PR5, PR6, PR7' option

** Marine version – CL1: Devices with 'Extended tower length – TE3' option

Figure 5: Remote mount design

... Flowmeter sensor

... Dimensions

Devices DN 15 to 150 in NAMUR standard installation lengths

Meter tube	Process connection EN 1092-1 B1	L	Ø k	Ø A	B	C	E	E1	Approximate weight
DN 15 (½ in)	DN 15 (½ in) / PN 40	510 (20.08) ¹⁾	60 (2.4)	44.5 (1.8)	77 (3.0)	46 (1.8)	283 (11.1)	283 (11.1)	13.5
							410* (16.1*)	357** (14.1**) (29.8)	
DN 25 (1 in)	DN 25 (1 in) / PN 40	600 (23.62) ¹⁾	75 (3.0)	69.5 (2.74)	103 (4.06)	62 (2.44)	324 (12.8)	324 (12.8)	15
							451* (17.8*)	398** (15.7**) (33.1)	
DN 50 (1 in)	DN 50 (1 in) / PN 40	715 (28.15) ¹⁾	125 (4.92)	99 (3.9)	125 (4.92)	80 (3.15)	354 (13.9)	354 (13.9)	31
							481* (18.94*)	428** (16.9**) (68.3)	
DN 80 (3 in)	DN 80 (3 in) / PN 40	915 (36.02) ¹⁾	160 (6.30)	155 (6.1)	183 (7.2)	123 (4.84)	445 (17.52)	–	74
							572* (22.52*)		(163)
DN 100 (4 in)	DN 100 (4 in) / PN 16	1400 (55.12) ²⁾	180 (7.09)	195 (7.68)	261 (10.28)	168 (6.61)	541 (21.3)	–	123
							668* (26.3*)		(271)
DN 150 (6 in)	DN 150 (6 in) / PN 16	1700 (66.93) ³⁾	240 (9.45)	260 (10.24)	320 (12.6)	205 (8.07)	630 (24.8)	–	178
							757* (29.8*)		(392)

* Standard design: Devices with 'Extended tower length – TE1, TE2' option or 'Pressure rating of sensor secondary housing' option

** Marine version – CL1: Devices with 'Extended tower length – TE3' option

L dimension tolerances

1) +0 / -3 mm (+0 / -0.118 in)


2) +0 / -5 mm (+0 / -0.20 in)

3) +0 / -20 mm (+0 / -0.79 in)

Devices with meter tube nominal diameter DN 15 to 80 and connections in accordance with SMS 1145, DIN 11851, DIN 32676, DIN ISO 228, ASME BPE and ASME B 1.20.1

Sensor with wetted parts made from stainless steel.

All dimensions and weights are specified in mm (in) or kg (lb).

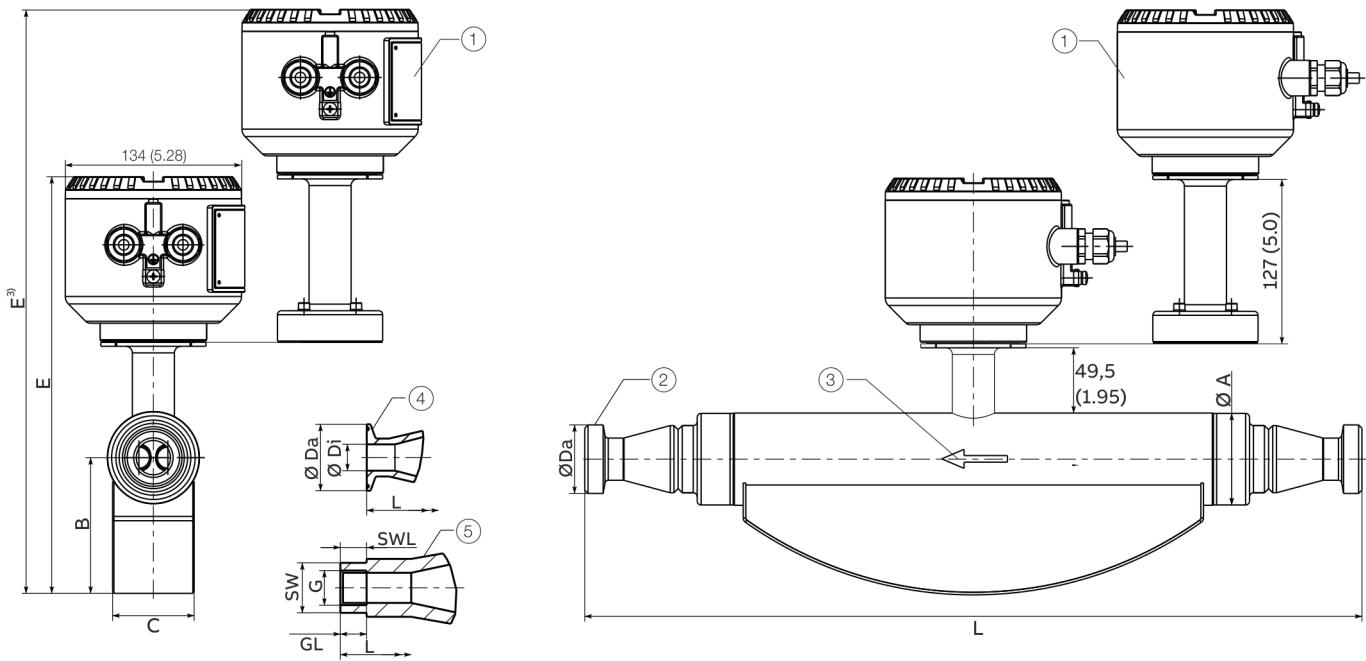

- (1) 'Extended tower length – TE1, TE2' option or 'Pressure rating of sensor secondary housing – PR5, PR6, PR7' option
- (2) Threaded spuds in accordance with DIN 11851 and SMS 1145
- (3) Flow direction
- (4) Clamping connection in accordance with DIN 32676 and ASME BPE
- (5) Female thread connection in accordance with DIN ISO 228 and ASME B 1.20.1

Figure 6: Remote mount design

Process connection in accordance with SMS 1145 meter tube nominal diameter DN 25 to 80 (1 to 3 in)

Meter tube	Process connection	L	Ø DA	Ø Di	Ø A	B	C	E	Approximate weight
DN	DN	PN							Aluminum* Stainless steel**
25 (1 in)	25 (1 in)	6	590 (23.2)	RD 40x1/8 in	22.6 (0.89)	69.5	103	62	317 / 444***
	40 (1 1/2 in)			RD 60x1/8 in	38 (1.50)	(2.74)	(4.06)	(2.44)	(12.48 / 17.48***)
50 (2 in)	40 (1 1/2 in)	6	763 (30.0)	RD 60x1/8 in	35.5 (1.40)	99	125	80	354 / 481***
	50 (2 in)		740 (29.1)	RD 70x1/8 in	48.5 (1.91)	(3.46)	(4.92)	(3.15)	(13.94 / 18.94***)
	65 (2 1/2 in)			RD 85x1/8 in	60.5 (2.38)				
80 (3 in)	65 (2 1/2 in)	990 (39.0)	RD 85x1/8 in	60.5 (2.38)	155	183	123	445 / 572***	68 / 69***
	80 (3 in)	940 (37.0)	RD 98x1/4 in	72.6 (2.86)	(6.10)	(7.20)	(4.84)	(17.52 / 22.52***)	(150 / 152***)
* Devices with terminal boxes made from aluminum.									
** Devices with terminal boxes made from stainless steel.									
*** Devices with 'Extended tower length' option or 'Pressure rating of sensor secondary housing' option.									

* Devices with terminal boxes made from aluminum.

** Devices with terminal boxes made from stainless steel.

*** Devices with 'Extended tower length' option or 'Pressure rating of sensor secondary housing' option.

... Flowmeter sensor

... Dimensions

Process connection in accordance with DIN 11851 meter tube nominal diameter DN 15 to 80 (½ to 3 in.)

Meter tube	Process connection		L	Ø DA	Ø Di	Ø A	B	C	E	Approximate weight	
DN	DN	PN								Aluminum*	Stainless steel**
15 (½ in)	10 (⅜ in)	40	413 (16.3)	RD 28x⅛ in	10 (0.39)	44.5	77 (3.03)	46 (1.81)	278 / 405***	9 / 10***	12 / 13***
	15 (½ in)			RD 34x⅛ in	16 (0.63)	(1.75)			(10.94 / 15.94***)	(20 / 22***)	(27 / 29***)
	20 (¾ in)			RD 44x⅛ in	20 (0.79)						
25 (1 in)	20 (¾ in)	590 (23.2)	RD 44x⅛ in	20 (0.79)	69.5	103	62	317 / 444***	11 / 12***	14 / 15***	
	25 (1 in)		RD 52x⅛ in	26 (1.02)	(2.74)	(4.06)	(2.44)	(12.48 / 17.48***)	(24 / 27***)	(31 / 33***)	
	40 (1 ½ in)		RD 65x⅛ in	38 (1.5)							
50 (2 in)	40 (1 ½ in)	763 (30.0)	RD 65x⅛ in	38 (1.5)	99 (3.46)	125	80	354 / 481***	27 / 28***	30 / 31***	
	50 (2 in)	25	740 (29.1)	RD 78x⅛ in	50 (1.97)	(4.92)	(3.15)	(13.94 / 18.94***)	(60 / 62***)	(66 / 68***)	
	65 (2 ½ in)		RD 95x⅛ in	66 (2.6)							
80 (3 in)	65 (2 ½ in)	990 (39.0)	RD 95x⅛ in	66 (2.6)	155	183	123	445 / 572***	68 / 69***	71 / 72***	
	80 (3 in)		RD 110x⅔ in	81 (3.19)	(6.10)	(7.20)	(4.84)	(17.52 / 22.52***)	(150 / 152***)	(157 / 159***)	
	100 (4 in)		RD 130x⅔ in	100 (3.94)							

Process connection in accordance with DIN 32676 meter tube nominal diameter DN 15 to 80 (½ to 3 in.)

Meter tube	Process connection		L	Ø DA	Ø Di	Ø A	B	C	E	Approximate weight	
DN	DN	PN								Aluminum*	Stainless steel**
15 (½ in)	10 (⅜ in)	40	413 (16.3)	34 (1.34)	10 (0.39)	44.5	77 (3.03)	46 (1.81)	278 / 405***	9 / 10***	12 / 13***
	15 (½ in)				16 (0.63)	(1.75)			(10.94 / 15.94***)	(20 / 22***)	(27 / 29***)
	20 (¾ in)				20 (0.79)						
25 (1 in)	20 (¾ in)	590 (23.2)			20 (0.79)	69.5	103	62	317 / 444***	11 / 12***	14 / 15***
	25 (1 in)		50.5 (1.99)	26 (1.02)	(2.74)	(4.06)	(2.44)	(12.48 / 17.48***)	(24 / 27***)	(31 / 33***)	
	40 (1 ½ in)				38 (1.5)						
50 (2 in)	40 (1 ½ in)	763 (30.0)			38 (1.5)	99 (3.46)	125	80	354 / 481***	27 / 28***	30 / 31***
	50 (2 in)	25	740 (29.1)	64 (2.52)	50 (1.97)	(4.92)	(3.15)	(13.94 / 18.94***)	(60 / 62***)	(66 / 68***)	
	65 (2 ½ in)		91 (3.58)	66 (2.6)							
80 (3 in)	65 (2 ½ in)	10	950 (37.4)		66 (2.6)	155	183	123	445 / 572***	68 / 69***	71 / 72***
	80 (3 in)		910 (35.83)	106 (4.17)	81 (3.19)	(6.10)	(7.20)	(4.84)	(17.52 / 22.52***)	(150 / 152***)	(157 / 159***)
	100 (4 in)			119 (4.69)	100 (3.94)						

* Devices with terminal boxes made from aluminum.

** Devices with terminal boxes made from stainless steel.

*** Devices with 'Extended tower length' option or 'Pressure rating of sensor secondary housing' option.

Tolerance for dimension L: +0 / -3 mm (+0 / -0.118 in)

Dimensions for sensors featuring meter tubes with nominal diameter DN 15 to 80 ($\frac{1}{2}$ to 3 in.) and process connection in accordance with ASME BPE											
Meter tube	Process connection		L	\varnothing DA	\varnothing Di	\varnothing A	B	C	E	Approximate weight	
DN	DN	PN								Aluminum ¹	Stainless steel ²
15 ($\frac{1}{2}$ in)	$\frac{3}{8}$ in-Type A	10	—	—	—	44.5	77 (3.03)	46 (1.81)	278 / 405 ³	9 / 10 ³	12 / 13 ³
	$\frac{1}{2}$ in-Type A	433 (17.05)	25 (0.98)	9.4 (0.37)	(1.75)				(10.94 / 15.94 ³)	(20 / 22 ³)	(27 / 29 ³)
	$\frac{3}{4}$ in-Type A	—	—	—	—						
25 (1 in)	$\frac{3}{4}$ in-Type A	—	—	—	—	69.5	103	62	317 / 444 ³	11 / 12 ³	14 / 15 ³
	1 in-Type B	590 (23.23)	50.4 (1.98)	22.1 (0.87)	(2.74)	(4.06)	(2.44)		(12.48 / 17.48 ³)	(24 / 27 ³)	(31 / 33 ³)
	1 $\frac{1}{2}$ in-Type B	590 (23.23)	50.4 (1.98)	34.8 (1.37)							
50 (2 in)	1 $\frac{1}{2}$ in-Type B	—	—	—	99 (3.46)	125	80		354 / 481 ³	27 / 28 ³	30 / 31 ³
	2 in-Type B	740 (29.13)	63.9 (2.52)	47.5 (1.87)		(4.92)	(3.15)		(13.94 / 18.94 ³)	(60 / 62 ³)	(66 / 68 ³)
	2 $\frac{1}{2}$ in-Type B	—	—	—							
80 (3 in)	2 $\frac{1}{2}$ in-Type B	950 (37.40)	77.4 (3.05)	60.2 (2.37)		155	183	183	445 / 572 ³	68 / 69 ³	71 / 72 ³
	3 in-Type B	910 (35.83)	90.9 (3.19)	72.9 (2.87)	(6.10)	(7.20)	(7.20)		(17.52 / 22.52 ³)	(150 / 152 ³)	(157 / 159 ³)
	4 in-Type B	910 (35.83)	118.9 (4.68)	97.4 (3.83)							

Process connection in accordance with DIN ISO 228 and ASME B 1.20.1, meter tube nominal diameter DN 15 ($\frac{1}{2}$ in)

Meter tube	Process connection		L	GL ⁴	WS ⁵	SWL ⁵	\varnothing A	B	C	E	Approximate weight	
DN	DN / G	PN									Aluminum ¹	Stainless steel ²
15 ($\frac{1}{2}$ in)	8 ($\frac{1}{4}$ in) / G $\frac{1}{4}$ in	100	450	10 (0.39) (17.72)	19	10 (0.39)	44.5	77 (3.03)	46 (1.81) (1.75)	278 / 405 ³ (10.94 / 15.94 ³)	9 / 10 ³ (20 / 22 ³)	12 / 13 ³ (27 / 29 ³)
	15 ($\frac{1}{2}$ in) / G $\frac{1}{2}$ in			13.5 (0.53)	27	15 (0.59)						
	25 (1 in) / G 1 in		490	17 (0.67) (19.29)	50	20 (0.79)						
	15 ($\frac{1}{2}$ in) / $\frac{1}{2}$ in NPT		450	15.6 (0.61) (17.72)	27	15 (0.59)						

¹ Devices with terminal boxes made from aluminum.² Devices with terminal boxes made from stainless steel.³ Devices with 'Extended tower length' option or 'Pressure rating of sensor secondary housing' option.⁴ Dimension GL: Provide thread length of female thread.⁵ Dimension SW: Provide width across flats in mm, Dimension SWL: Provide length of wrench flats in mm.

Tolerance for dimension L: +0 / -3 mm (+0 / -0.118 in)

... Flowmeter sensor

... Dimensions

Sensor with wetted parts made from C4 or C22 nickel alloy

For devices with wetted parts made from C4 or C22 nickel alloy, the installation length (L) is different from previous tables. All other dimensions and the weight are unchanged.

Dimensions in mm (in).

Dimensions for sensors with process connection in accordance with EN 1092-1 and ASME B16.5 (ANSI)									
Meter tube nominal diameter	Process connection	L EN 1092-1 B1 PN 16	L EN 1092-1 B1 PN 40	L EN 1092-1 B2 PN 63	L EN 1092-1 B2 PN 100	L ASME CL150	L ASME CL300	L ASME CL600	L JIS 10K
DN 15 (½ in)	DN 10 (¼ in)	—	449 (17.7)	449 (17.7)	449 (17.7)	—	—	—	449 (17.7)
	DN 15 (½ in)	—	442 (17.4)	442 (17.4)	442 (17.4)	442 (17.4)	442 (17.4)	442 (17.4)	442 (17.4)
	DN 20 (¾ in)	—	428 (16.9)	428 (16.9)	428 (16.9)	428 (16.9)	428 (16.9)	428 (16.9)	428 (16.9)
DN 25 (1 in)	DN 20 (¾ in)	—	646 (25.4)	646 (25.4)	646 (25.4)	646 (25.4)	646 (25.4)	646 (25.4)	646 (25.4)
	DN 25 (1 in)	—	614 (24.2)	614 (24.2)	614 (24.2)	614 (24.2)	614 (24.2)	614 (24.2)	614 (24.2)
	DN 40 (1½ in)	—	576 (22.7)	576 (22.7)	576 (22.7)	576 (22.7)	576 (22.7)	576 (22.7)	576 (22.7)
DN 50 (2 in)	DN 40 (1½ in)	—	814 (32.0)	814 (32.0)	814 (32.0)	814 (32.0)	814 (32.0)	814 (32.0)	814 (32.0)
	DN 50 (2 in)	—	764 (30.1)	764 (30.1)	764 (30.1)	764 (30.1)	764 (30.1)	764 (30.1)	764 (30.1)
	DN 65 (2½ in)	—	819 (32.2)	819 (32.2)	819 (32.2)	792 (31.2)	792 (31.2)	792 (31.2)	819 (32.2)
DN 80 (3 in)	DN 65 (2½ in)	—	1021 (40.2)	1021 (40.2)	1021 (40.2)	1021 (40.2)	1021 (40.2)	1021 (40.2)	1021 (40.2)
	DN 80 (3 in)	—	971 (38.2)	—	971 (38.2)	971 (38.2)	971 (38.2)	971 (38.2)	971 (38.2)
	DN 100 (4 in)	971 (38.2)	971 (38.2)	971 (38.2)	971 (38.2)	971 (38.2)	971 (38.2)	971 (38.2)	971 (38.2)
DN 100 (4 in)	DN 80 (3 in)	1357 (53.4)	1357 (53.4)	1357 (53.4)	1357 (53.4)	1357 (53.4)	1357 (53.4)	1357 (53.4)	1357 (53.4)
	DN 100 (4 in)	1280 (50.4)	1280 (50.4)	1280 (50.4)	1280 (50.4)	1280 (50.4)	1280 (50.4)	1280 (50.4)	1280 (50.4)
	DN 150 (6 in)	1261 (49.6)	1261 (49.6)	1261 (49.6)	1261 (49.6)	1261 (49.6)	1261 (49.6)	1261 (49.6)	1261 (49.6)
DN 150 (6 in)	DN 100 (4 in)	1592 (62.7)	1592 (62.7)	1632 (64.3)	1632 (64.3)	1592 (62.7)	1632 (64.3)	1632 (64.3)	1592 (62.7)
	DN 150 (6 in)	1502 (59.1)	1502 (59.1)	1542 (60.7)	1542 (60.7)	1502 (59.1)	1542 (60.7)	1542 (60.7)	1502 (59.1)

L dimension tolerance:

- Meter tube nominal diameter DN 15 to 50 (½ to 2 in): +0 / -3 mm (+0 / -0.118 in)
- Meter tube nominal diameter DN 80 (3 in): +0 / -5 mm (+0 / -0.197 in)
- Meter tube nominal diameter DN 100 (4 in): +0 / -15 mm (+0 / -0.59 in)
- Meter tube nominal diameter DN 150 (6 in): +0 / -20 mm (+0 / -0.79 in)

Ordering information

Note

For additional information on dependencies and restrictions, and for help on product selection, please refer to the Online Product Selection Assistant (PSA) at www.abb.us/flow-selector.

CoriolisMaster FCB130, FCB150

CoriolisMaster FCB130 Coriolis Mass Flowmeter	FCB130	XX	XX	XXXXX	XX	XX	X	X	XX	XX	X
CoriolisMaster FCB150 Coriolis Mass Flowmeter	FCB150	XX	XX	XXXXX	XX	XX	X	X	XX	XX	X
Explosion Protection Certification											
General Purpose				Y0							
ATEX / IECEx (Zone 2 / 22)				A2							
ATEX / IECEx (Zone 1 / 21)				A1							
cFMus version Class 1 Div. 2 (Zone 2 / 21)				F2							
cFMus version Class 1 Div. 1 (Zone 1 / 21)				F1							
UKEX (Zone 2 / 22)				U2							
UKEX (Zone 1 / 21)				U1							
Connection Design / Connection Box Material / Cable Glands											
Integral, defined by Transmitter housing				Y0							
Meter Size / Connection Size											
DN 15 (½ in) / DN 10 ¾ in					015E1						
DN 15 (½ in) / DN 15 (½ in)					015R0						
DN 15 (½ in) / DN 20 (¾ in)					015R1						
DN 25 (1 in) / DN 20 (¾ in)					025E1						
DN 25 (1 in) / DN 25 (1 in)					025R0						
DN 25 (1 in) / DN 40 (1½ in)					025R2						
DN 50 (2 in) / DN 40 (1½ in)					050E1						
DN 50 (2 in) / DN 50 (2 in)					050R0						
DN 50 (2 in) / DN 65 (2½ in)					050R1						
DN 80 (3 in) / DN 65 (2½ in)					080E1						
DN 80 (3 in) / DN 80 (3 in)					080R0						
DN 80 (3 in) / DN 100 (4 in)					080R1						
DN 100 (4 in) / DN 80 (3 in)					100E1						
DN 100 (4 in) / DN 100 (4 in)					100R0						
DN 100 (4 in) / DN 150 (6 in)					100R2						
DN 150 (6 in) / DN 100 (4 in)					150E2						
DN 150 (6 in) / DN 150 (6 in)					150R0						
DN 150 (6 in) / DN 200 (8 in)					150R2						

Continuation see next page

... Flowmeter sensor

... Ordering information

Base model

CoriolisMaster FCB130 Coriolis Mass Flowmeter	XX	XX	X	X	XX	XX	X
CoriolisMaster FCB150 Coriolis Mass Flowmeter	XX	XX	X	X	XX	XX	X

Process Connection Type

Flanges DIN PN 16	D2						
Flanges DIN PN 40	D4						
Flanges DIN PN 63	D5						
Flanges DIN PN 100	D6						
Flanges EN 1092-1 PN 40, NAMUR length (DN 15, DN 25, DN 50, DN 80)	S5						
Flanges with groove PN40 EN1092-10-D	S6						
Flanges EN 1092-1 PN 16, NAMUR length (DN 100, DN 150)	S7						
Flanges ANSI / ASME B16.5 Class 150	A1						
Flanges ANSI / ASME B16.5 Class 300	A3						
Flanges ANSI / ASME B16.5 Class 600	A6						
Flanges ANSI / ASME B16.5 Class 900 (p-t rating Cl 600)	A7						
Flanges ANSI / ASME B16.5 Class 1500 (p-t rating Cl 600)	A8						
Flanges JIS 10K	J1						
Flanges JIS 20K	J3						
Threaded hygienic connection SMS1145, for pipe according to DIN11866 series A	K1						
Tri-Clamp acc. DIN 32676	T1						
Tri-Clamp acc. BPE	T3						
Food industry fittings acc. DIN 11851	F1						
Female NPT thread	N5						
Female G thread	M5						
Others	Z9						

Material of Wetted Parts

Stainless steel	A1						
Ni-Alloy	C1*						

Flow Calibration

Flow forward ±0.40 % of flow rate, Gas 1 % of flow rate	A**						
Flow forward ±0.25 % of flow rate, Gas 1 % of flow rate	B**						
Flow forward ±0.15 % of flow rate, Gas 0.5 % of flow rate	C***						
Flow forward ±0.10 % of flow rate, Gas 0.5 % of flow rate	D***						
Flow forward ±0.20 % of flow rate, Gas 1 % of flow rate	E**						
Flow forward / reverse ±0.40 % of flow rate, Gas 1 % of flow rate	J**						
Flow forward / reverse ±0.25 % of flow rate, Gas 1 % of flow rate	K**						
Flow forward / reverse ±0.15 % of flow rate, Gas 0.5 % of flow rate	L***						
Flow forward / reverse ±0.10 % of flow rate, Gas 0.5 % of flow rate	M***						
Flow forward / reverse ±0.20 % of flow rate, Gas 1 % of flow rate	N***						
Others	Z						

Density Calibration

Density 10 g/l	1**						
Density 2 g/l	3***						
Density 1 g/l	4***						
Density 0,4 g/l	5***						
Others	9						

* If the sensor wetted parts are Ni-Alloy based, parts of the sensor housing are Ni-Alloy

** Only with CoriolisMaster FCB130

*** Only with CoriolisMaster FCB150

Continuation see next page

Base model

CoriolisMaster FCB130 Coriolis Mass Flowmeter	XX	XX	X
CoriolisMaster FCB150 Coriolis Mass Flowmeter	XX	XX	X

Connection Design / Transmitter Housing Type / Transmitter Housing Material / Cable Glands

Integral / Single compartment / Aluminum / 2 × M20 × 1,5	B1
Integral / Single compartment / Aluminum / 2 × NPT ½ in	B2
Integral / Single compartment / Stainless Steel / 2 × M20 × 1,5	T1
Integral / Single compartment / Stainless Steel / 2 × NPT ½ in	T2

Outputs

MODBUS, 2 digital outputs (passive)	M2
-------------------------------------	----

Power Supply

11 to 30 V DC	C
---------------	---

Additional ordering information

CoriolisMaster FCB130 Coriolis Mass Flowmeter	XX	XXX	XXX	XXX	XX
CoriolisMaster FCB150 Coriolis Mass Flowmeter	XX	XXX	XXX	XXX	XX

Certificates

Test report 2.2 acc. EN 10204 confirmation of material	C1
Material monitoring with inspection certificate 3.1 acc. EN 10204	C2
Material monitoring with inspection certificate 3.2 acc. EN 10204	C3
Material monitoring NACE MR 01-75 with inspection certificate 3.1 acc. EN 10204	CN
Declaration of compliance with the order 2.1 acc. EN 10204	C4
Inspection certificate 3.1 acc. EN 10204 for visual, dimensional and functional test	C6
Inspection certificate 3.1 acc. EN 10204 for positive material identification PMI (confirmation only)	CA
Pressure test acc. AD2000	CB
Test package (pressure test, non-destructive test, welder & welding procedure certificate)	CT
Inspection certificate 3.1 acc. EN 10204 for NDE of welds	C8
Certificate of accuracy 2.1 acc. EN 10204	CM
Inspection certificate 3.1 acc. EN 10204 for positive material identification PMI (inclusive heat analysis)	CR
Others	CZ

Other Usage Certifications

UKCA conformity	CU1
-----------------	-----

Ships Register Certifications

DNVG	CL1
------	-----

Custody Transfer Certification

Custody transfer acc. MID (OIML CI 0.5/0.3))	CT3*
Custody transfer acc. MID (OIML CI 0.5)	CT4*

Special Operation Mode

Standard + FillMass filling function	N5*
Standard + DensiMass concentration measurement	N6*
VeriMass - Meter verification	N7

* Only with CoriolisMaster FCB150

Continuation see next page

... Flowmeter sensor

... Ordering information

Additional ordering information

CoriolisMaster FCB130 Coriolis Mass Flowmeter	XX	XXX	XX	XXX
CoriolisMaster FCB150 Coriolis Mass Flowmeter	XX	XXX	XX	XXX
Documentation Language				
German	M1			
English	M5			
Language package Western Europe / Scandinavia (Languages: DA, ES, FR, IT, NL, PT, FI, SV)	MW			
Language package Eastern Europe (Languages: EL, CS, ET, LV, LT, HU, HR, PL, SK, SL, RO, BG)	ME			
Others	MZ			
Pressure Rating of Sensor Secondary Containment				
Maximum burst pressure 6 MPa / 60 bar / 870 psi inclusive tower length extension	PR5			
Maximum burst pressure 10 MPa / 100 bar / 1450 psi inclusive tower length extension	PR6			
Maximum burst pressure 15 MPa / 150 bar / 2175 psi inclusive tower length extension	PR7			
Device Identification Plate				
Stainless steel plate with TAG no.	T1			
Others	TZ			
Extended Tower Length				
Tower length extension - meter insulation capability	TE1			
Tower length extension - meter insulation capability with double sealing	TE2			
Tower length extension -short- insulation capability	TE3			

Accessories

Description	Order number
FCx1xx Local Operation Interface (LOI) adapter and cable	3KXS310000L0001

Note

For additional information on dependencies and restrictions, and for help on product selection, please refer to the Online Product Selection Assistant (PSA) at www.abb.us/flow-selector.

CoriolisMaster FCH130, FCH150

Base model		FCH130	XX	XX	XXXXX	XX	XX	X	X	XX	XX	X
CoriolisMaster FCH130 Coriolis Mass Flowmeter		FCH130	XX									
CoriolisMaster FCH150 Coriolis Mass Flowmeter		FCH150	XX	XX	XXXXX	XX	XX	X	X	XX	XX	X
Explosion Protection Certification												
General Purpose				Y0								
ATEX / IECEx (Zone 2 / 22)				A2								
ATEX / IECEx (Zone 1 / 21)				A1								
cFMus version Class 1 Div. 2 (Zone 2 / 21)				F2								
cFMus version Class 1 Div. 1 (Zone 1 / 21)				F1								
UKEX (Zone 2 / 22)				U2								
UKEX (Zone 1 / 21)				U1								
Connection Design / Connection Box Material / Cable Glands												
Integral, defined by Transmitter housing							Y0					
Meter Size / Connection Size												
DN 25 (1 in) / DN 20 (¾ in)								025E1				
DN 25 (1 in) / DN 25 (1 in)								025R0				
DN 25 (1 in) / DN 40 (1½ in)								025R2				
DN 50 (2 in) / DN 40 (1½ in)								050E1				
DN 50 (2 in) / DN 50 (2 in)								050R0				
DN 50 (2 in) / DN 65 (2½ in)								050R1				
DN 80 (3 in) / DN 65 (2½ in)								080E1				
DN 80 (3 in) / DN 80 (3 in)								080R0				
DN 80 (3 in) / DN 100 (4 in)								080R1				
Process Connection Type												
Tri-Clamp acc. DIN 32676									T1			
Tri-Clamp acc. BPE									T3			
Food industry fittings acc. DIN 11851									F1			
Others									Z9			
Material of Wetted Parts												
Stainless steel AISI 316L (1.4404), polished									H2			

Continuation see next page

... Flowmeter sensor

... Ordering information

Base model

CoriolisMaster FCH130 Coriolis Mass Flowmeter	X	X	XX	XX	X
CoriolisMaster FCH150 Coriolis Mass Flowmeter	X	X	XX	XX	X

Flow Calibration

Flow forward ±0.40 % of flow rate, Gas 1 % of flow rate	A*
Flow forward ±0.25 % of flow rate, Gas 1 % of flow rate	B*
Flow forward ±0.15 % of flow rate, Gas 0.5 % of flow rate	C**
Flow forward ±0.10 % of flow rate, Gas 0.5 % of flow rate	D**
Flow forward ±0.20 % of flow rate, Gas 1 % of flow rate	E*
Flow forward / reverse ±0.40 % of flow rate, Gas 1 % of flow rate	J*
Flow forward / reverse ±0.25 % of flow rate, Gas 1 % of flow rate	K*
Flow forward / reverse ±0.15 % of flow rate, Gas 0.5 % of flow rate	L**
Flow forward / reverse ±0.10 % of flow rate, Gas 0.5 % of flow rate	M**
Flow forward / reverse ±0.20 % of flow rate, Gas 1 % of flow rate	N*
Others	Z

Density Calibration

Density 10 g/l	1*
Density 2 g/l	3**
Density 1 g/l	4**
Density 0,4 g/l	5**
Others	9

Connection Design / Transmitter Housing Type / Transmitter Housing Material / Cable Glands

Integral / Single compartment / Aluminum / 2 x M20 x 1.5	B1
Integral / Single compartment / Aluminum / 2 x NPT ½ in.	B2
Integral / Single compartment / Stainless Steel / 2 x M20 x 1.5	T1
Integral / Single compartment / Stainless Steel / 2 x NPT ½ in.	T2

Outputs

MODBUS, 2 digital outputs (passive)	M2
-------------------------------------	----

Power Supply

11 to 30 V DC	C
---------------	---

* Only with CoriolisMaster FCH130

** Only with CoriolisMaster FCH150

Continuation see next page

Additional ordering information

CoriolisMaster FCH130 Coriolis Mass Flowmeter	XX	XXX	XXX	XX	XX	XX	XXX
CoriolisMaster FCH150 Coriolis Mass Flowmeter	XX	XXX	XXX	XX	XX	XX	XXX
Certificates							
Test report 2.2 acc. EN 10204 confirmation of material	C1						
Material monitoring with inspection certificate 3.1 acc. EN 10204	C2						
Material monitoring with inspection certificate 3.2 acc. EN 10204	C3						
Material monitoring NACE MR 01-75 with inspection certificate 3.1 acc. EN 10204	CN						
Declaration of compliance with the order 2.1 acc. EN 10204	C4						
Inspection certificate 3.1 acc. EN 10204 for visual, dimensional and functional test	C6						
Inspection certificate 3.1 acc. EN 10204 for positive material identification PMI (confirmation only)	CA						
Pressure test acc. AD2000	CB						
Test package (pressure test, non-destructive test, welder & welding procedure certificate)	CT						
Inspection certificate 3.1 acc. EN 10204 for NDE of welds	C8						
Certificate of accuracy 2.1 acc. EN 10204	CM						
Inspection certificate 3.1 acc. EN 10204 for positive material identification PMI (inclusive heat analysis)	CR						
Others	CZ						
Other Usage Certifications							
UKCA conformity	CU1						
Hygienic Approval							
EHEDG	CWL*						
Special Operation Mode							
Standard + FillMass filling function	N5**						
Standard + DensiMass concentration measurement	N6**						
VeriMass - Meter verification	N7						
Documentation Language							
German	M1						
English	M5						
Language package Western Europe / Scandinavia (Languages: DA, ES, FR, IT, NL, PT, FI, SV)	MW						
Language package Eastern Europe (Languages: EL, CS, ET, LV, LT, HU, HR, PL, SK, SL, RO, BG)	ME						
Others	MZ						
Device Identification Plate							
Stainless steel plate with TAG no.	T1						
Others	TZ						
Extended Tower Length							
Tower length extension - meter insulation capability	TE1						
Tower length extension - meter insulation capability with double sealing	TE2						

* EHEDG (optional), FDA-konform

** Only with CoriolisMaster FCH150

Accessories

Description	Order number
FCx1xx Local Operation Interface (LOI) adapter and cable	3KXS310000L0001





Use in potentially explosive atmospheres

Note





Further information on the approval of devices for use in potentially explosive atmospheres can be found in the type examination certificates or the relevant certificates at www.abb.com/flow.

Device overview

ATEX, IECEx and UKEX

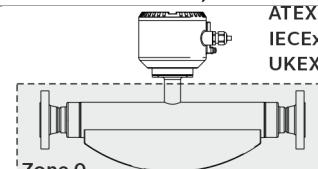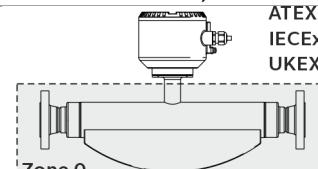Model number	Standard / No explosion protection FCx1xx Y0	Zone 2, 21, 22 FCx1xx A2, U2	Zone 1, 21 (Zone 0) FCx1xx A1, U1
<ul style="list-style-type: none"> • Standard • Zone 2, 21, 22 • Zone 1, 21 • Zone 0 			

cFMus

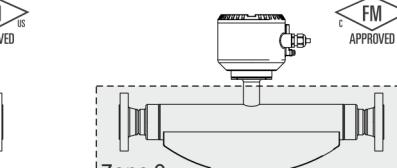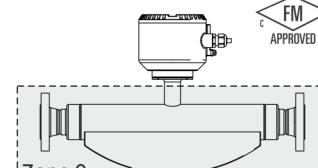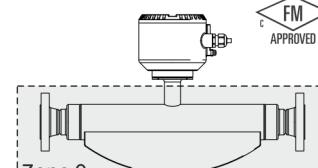Model number	Standard / No explosion protection FCx1xx Y0	Class I Div. 2 Zone 2, 21 FCx1xx F2	Class I Div. 1 Zone 0, 1, 20 ,21 FCx1xx F1
<ul style="list-style-type: none"> • Standard • Class I Div. 2 • Class I Div. 1 • Zone 2, 21 • Zone 1, 21 • Zone 0, 20 			

Ex marking

Note

- A specific marking applies, depending on the design.
- ABB reserves the right to modify the Ex-marking. Refer to the name plate for the exact marking.

ATEX, IECEx and UKEX

Model FCx1xx-A2, U2... in Zone 2, 21, 22

ATEX

Certificate (ATEX): FM 14 ATEX0017X
 Certificate (UKEX): FM22UKEX0041X
 II 3 G Ex ec mc IIC T6 ... T2 Gc
 FM 14 ATEX0016X
 II 2 D Ex tb IIIC T85°C ... T_{medium} Db

IECEx

Certificate: IECEEx FME 14.0003X
 Ex ec mc IIC T6 ... T2 Gc
 Ex tb IIIC T85°C ... T_{medium} Db

Model FCx1xx-A1, U1... in Zone 1, 21 (Zone 0)

ATEX

Certificate (ATEX): FM 14 ATEX0016X
 Certificate (UKEX): FM22UKEX0042X
 II 1/2 G Ex eb ia mb IIC T6 ... T2 Ga/Gb
 II 2 D Ex ia tb IIIC T85°C ... T_{medium} Db

IECEx

Certificate: IECEEx FME 14.0003X
 Ex eb ia mb IIC T6 ... T2 Ga/Gb T_{amb,max}= 70°C
 Ex ia tb IIIC T85°C ... T_{medium} Db

cFMus

Model FCx1xx-F2... in Zone 2, Div. 2

FM (marking US)

Certificate: FM16US0201X
 NI: CL I, DIV2, GPS ABCD, T6 ... T2
 NI: CL II, III, DIV2, GPS EFG, T6 ... T3B
 DIP: CL II, Div 1, GPS EFG, T6 ... T3B
 DIP: CL III, Div 1, 2, T6 ... T3B
 CL I, ZN 2, AEx ec IIC T6 ... T2 Gc
 ZN 21 AEx tb IIIC T85°C ... T165°C Db
 See Instructions for temperature class information

FM (marking Canada)

Certificate: FM16CA0104X
 NI: CL I, DIV2, GPS ABCD, T6 ... T2
 NI: CL II, III, DIV2, GPS EFG, T6 ... T3B
 DIP: CL II, Div 1, GPS EFG, T6 ... T3B
 DIP: CL III, Div 1, 2, T6 ... T3B
 Ex ec IIC T6 ... T2 Gc
 See Instructions for temperature class information

Model FCx1xx-F1... in Zone 1, Div. 1

FM (marking US)

Certificate: FM16US0201X
 XP-IS: CL I, Div 1, GPS BCD, T6 ... T2
 DIP: CL II, Div 1, GPS EFG, T6 ... T3B
 DIP: CL III, Div 1, 2, T6 ... T3B
 CL I, ZN 1, AEx db ia IIB+H2 T6 ... T2 Ga/Gb
 ZN 21 AEx ia tb IIIC T85°C to T165°C Db
 See Instructions for temperature class information and Installation
 Drawing No. 3KXF000014G0009

FM (marking Canada)

Certificate: FM16CA0104X
 XP-IS: CL I, Div 1, GPS BCD, T6 ... T2
 DIP: CL II, Div 1, GPS EFG, T6 ... T2
 DIP: CL III, Div 1, 2, T6 ... T3B
 Ex db ia IIB+H2 T6 ... T2 Gb
 Ex ia INTRINSICALLY SAFE SECURITE INTRINSEQU
 See Instructions for temperature class information and Installation
 Drawing No. 3KXF000014G0009

... Use in potentially explosive atmospheres

Temperature data

Temperature resistance for the connecting cable

The temperature at the cable entries of the device is dependent on the measuring medium temperature T_{medium} and the ambient temperature $T_{\text{amb.}}$.

For the electrical connection of the device, use only cables with sufficient temperature resistance in accordance with the table.

$T_{\text{amb.}}$	Temperature resistance for the connecting cable
$\leq 50^{\circ}\text{C}$ ($\leq 122^{\circ}\text{F}$)	$\geq 105^{\circ}\text{C}$ ($\geq 221^{\circ}\text{F}$)
$\leq 60^{\circ}\text{C}$ ($\leq 140^{\circ}\text{F}$)	$\geq 110^{\circ}\text{C}$ ($\geq 230^{\circ}\text{F}$)
$\leq 70^{\circ}\text{C}$ ($\leq 158^{\circ}\text{F}$)	$\geq 120^{\circ}\text{C}$ ($\geq 248^{\circ}\text{F}$)

From an ambient temperature of $T_{\text{amb.}} \geq 60^{\circ}\text{C}$ ($\geq 140^{\circ}\text{F}$) the wires in the terminal boxes must be additionally insulated using the enclosed silicone hoses.

Environmental and process conditions for model

FCx1xx...

Ambient temperature $T_{\text{amb.}}$	-20 to 70°C (-4 to 158°F)
	-40 to 70°C^* (-40 to 158°F^*)
Measuring medium temperature	-40 to 205°C
T_{medium}	(-40 to 400°F)
IP rating / NEMA rating	IP 65, IP 67 / NEMA 4X, Type 4X

* Optional, with order code 'Ambient temperature range – TA9'

Measuring medium temperature (Ex data) for model FCx1xx-A1, U1... in Zone 1

The table shows the maximum permissible measuring medium temperature as a function of ambient temperature and temperature class.

Ambient temperature T _{amb.}	Temperature class					
	T1	T2	T3	T4	T5	T6
≤ 30 °C (≤ 86 °F)	205 °C (400 °F)	205 °C (400 °F)	195 °C (383 °F)	130 °C (266 °F)	95 °C (203 °F)	80 °C (176 °F)
≤ 40 °C (≤ 104 °F)	205 °C (400 °F)	205 °C (400 °F)	195 °C (383 °F)	130 °C (266 °F)	95 °C (203 °F)	80 °C (176 °F)
≤ 50 °C (≤ 122 °F)	205 °C (400 °F)	205 °C (400 °F)	195 °C (383 °F)	130 °C (266 °F)	95 °C (203 °F)	80 °C (176 °F)
≤ 60 °C (≤ 140 °F)	205 °C (400 °F)	205 °C (400 °F)	195 °C (383 °F)	130 °C (266 °F)	95 °C (203 °F)	80 °C (176 °F)
≤ 70 °C (≤ 158 °F)	205 °C (400 °F)	205 °C (400 °F)	195 °C (383 °F)	130 °C (266 °F)	95 °C (203 °F)	80 °C (176 °F)

Measuring medium temperature (Ex data) for model FCx1xx-A2, U2... in Zone 2

The table shows the maximum permissible measuring medium temperature as a function of ambient temperature and temperature class.

Ambient temperature T _{amb.}	Temperature class					
	T1	T2	T3	T4	T5	T6
≤ 30 °C (≤ 86 °F)	205 °C (400 °F)*	205 °C (400 °F)*	195 °C (383 °F)*	130 °C (266 °F)*	95 °C (203 °F)*	80 °C (176 °F)
	195 °C (383 °F)	195 °C (383 °F)	130 °C (266 °F)	95 °C (203 °F)	80 °C (176 °F)	—
≤ 40 °C (≤ 104 °F)	205 °C (400 °F)*	205 °C (400 °F)*	195 °C (383 °F)*	130 °C (266 °F)*	95 °C (203 °F)*	—
	180 °C (356 °F)	180 °C (356 °F)	130 °C (266 °F)	95 °C (203 °F)	80 °C (176 °F)	—
≤ 50 °C (≤ 122 °F)	205 °C (400 °F)*	205 °C (400 °F)*	130 °C (266 °F)*	130 °C (266 °F)*	80 °C (176 °F)*	—
	140 °C (284 °F)	140 °C (284 °F)	130 °C (266 °F)	95 °C (203 °F)	60 °C (140 °F)	—
≤ 60 °C (≤ 140 °F)	205 °C (400 °F)*	205 °C (400 °F)*	130 °C (266 °F)*	130 °C (266 °F)*	—	—
	120 °C (248 °F)	120 °C (248 °F)	120 °C (248 °F)	95 °C (203 °F)	—	—
≤ 70 °C (≤ 158 °F)	180 °C (356 °F)*	180 °C (356 °F)*	130 °C (266 °F)*	130 °C (266 °F)*	—	—
	80 °C (176 °F)	80 °C (176 °F)	80 °C (176 °F)	80 °C (176 °F)	—	—

* Only with the 'Extended tower length – TE1, TE2 or TE3' order option

Measuring medium temperature (Ex data) for model FCx1xx-A1, U1... in Zone 21 and FCx1xx-A2, U2... in Zone 22

The table shows the maximum permissible measuring medium temperature as a function of ambient temperature and temperature class.

Ambient temperature T _{amb.}	Temperature class				
	T210 °C	T200 °C	T135 °C	T100 °C	T85°C
≤ 30 °C (≤ 86 °F)	195 °C (383 °F)	130 °C (266 °F)	95 °C (203 °F)	80 °C (176 °F)	80 °C (176 °F)
≤ 50 °C (≤ 122 °F)	140 °C (284 °F)	130 °C (266 °F)	95 °C (203 °F)	60 °C (140 °F)	—
≤ 60 °C (≤ 140 °F)	120 °C (248 °F)	120 °C (248 °F)	95 °C (203 °F)	—	—
≤ 70 °C (≤ 158 °F)	80 °C (176 °F)	80 °C (176 °F)	80 °C (176 °F)	—	—

... Use in potentially explosive atmospheres

... Temperature data

Measuring medium temperature (Ex data) for model FCx1xx-F1... in Class I Div. 1, Class I Zone 1

The table shows the maximum permissible measuring medium temperature as a function of ambient temperature and temperature class.

Ambient temperature T _{amb.}	Temperature class					
	T1	T2	T3	T4	T5	T6
≤ 30 °C (≤ 86 °F)	205 °C (400 °F)	205 °C (400 °F)	195 °C (383 °F)	130 °C (266 °F)	95 °C (203 °F)	80 °C (176 °F)
≤ 40 °C (≤ 104 °F)	205 °C (400 °F)	205 °C (400 °F)	195 °C (383 °F)	130 °C (266 °F)	95 °C (203 °F)	80 °C (176 °F)
≤ 50 °C (≤ 122 °F)	205 °C (400 °F)	205 °C (400 °F)	195 °C (383 °F)	130 °C (266 °F)	95 °C (203 °F)	80 °C (176 °F)
≤ 60 °C (≤ 140 °F)	205 °C (400 °F)	205 °C (400 °F)	195 °C (383 °F)	130 °C (266 °F)	95 °C (203 °F)	80 °C (176 °F)
≤ 70 °C (≤ 158 °F)	205 °C (400 °F)	205 °C (400 °F)	195 °C (383 °F)	130 °C (266 °F)	95 °C (203 °F)	80 °C (176 °F)

Measuring medium temperature (Ex data) for model FCx1xx-F2... in Class I Div. 2, Class I Zone 2

The table shows the maximum permissible measuring medium temperature as a function of ambient temperature and temperature class.

Ambient temperature T _{amb.}	Temperature class					
	T1	T2	T3	T4	T5	T6
≤ 30 °C (≤ 86 °F)	205 °C (400 °F)*	205 °C (400 °F)*	195 °C (383 °F)*	130 °C (266 °F)*	95 °C (203 °F)*	80 °C (176 °F)
	195 °C (383 °F)	195 °C (383 °F)	130 °C (266 °F)	95 °C (203 °F)	80 °C (176 °F)	—
≤ 40 °C (≤ 104 °F)	205 °C (400 °F)*	205 °C (400 °F)*	195 °C (383 °F)*	130 °C (266 °F)*	95 °C (203 °F)*	—
	180 °C (356 °F)	180 °C (356 °F)	130 °C (266 °F)	95 °C (203 °F)	80 °C (176 °F)	—
≤ 50 °C (≤ 122 °F)	205 °C (400 °F)*	205 °C (400 °F)*	130 °C (266 °F)*	130 °C (266 °F)*	80 °C (176 °F)*	—
	140 °C (284 °F)	140 °C (284 °F)	130 °C (266 °F)	95 °C (203 °F)	60 °C (140 °F)	—
≤ 60 °C (≤ 140 °F)	205 °C (400 °F)*	205 °C (400 °F)*	130 °C (266 °F)*	130 °C (266 °F)*	—	—
	120 °C (248 °F)	120 °C (248 °F)	120 °C (248 °F)	95 °C (203 °F)	—	—
≤ 70 °C (≤ 158 °F)	180 °C (356 °F)*	180 °C (356 °F)*	130 °C (266 °F)*	130 °C (266 °F)*	—	—
	80 °C (176 °F)	80 °C (176 °F)	80 °C (176 °F)	80 °C (176 °F)	—	—

* Only with the 'Extended tower length – TE1, TE2 or TE3' order option

Measuring medium temperature (Ex data) for model FCx1xx-F1... in Zone 21, Class II / III and FCx1xx-F2... in Zone 22, Class II / III

The table shows the maximum permissible measuring medium temperature as a function of ambient temperature and temperature class.

Ambient temperature T _{amb.}	Temperature class				
	T210 °C	T200 °C	T135 °C	T100 °C	T85°C
≤ 30 °C (≤ 86 °F)	195 °C (383 °F)	130 °C (266 °F)	95 °C (203 °F)	80 °C (176 °F)	80 °C (176 °F)
≤ 50 °C (≤ 122 °F)	140 °C (284 °F)	130 °C (266 °F)	95 °C (203 °F)	60 °C (140 °F)	—
≤ 60 °C (≤ 140 °F)	120 °C (248 °F)	120 °C (248 °F)	95 °C (203 °F)	—	—
≤ 70 °C (≤ 158 °F)	80 °C (176 °F)	80 °C (176 °F)	80 °C (176 °F)	—	—

Electrical data – ATEX, IECEX, UKEX and cFMus

Modbus outputs and digital outputs

Modell ATEX, IECEX, UKCA: FCx1xx-A1, U1..., FCx1xx-A2, U2...

Modell: cFMus: FCx1xx-F1..., FCx1xx-F2...

Outputs	Operating values				Type of protection							
	(general)		„ec“ / „NI“ (Zone 2 / Div. 2)		„eb“ / „XP“ (Zone 1 / Div. 1)		„ia“ / „IS“ (Zone 1 / Div. 1)					
	U _N [V]	I _N [mA]	U _N [V]	I _N [mA]	U _M [V]	I _M [mA]	U _O [V]	I _O [mA]	P _O [mW]	C _O [nF]	C _{O_pa} [nF]	L _O [μH]
Modbus, active	3	30	3	30	30	30	4,2	150	150	13900	—	20
Terminals A / B							U _i [V]	I _i [mA]	P _i [mW]	C _i [nF]	C _{i pa} [nF]	L _i [μH]
							4,2	150	150	13900	—	20
Digital output DO1, passive	30	25	30	25	30	25	30	25	187	2,4	—	200
Terminals 41 / 42												
Digital output DO2, passive	30	25	30	25	30	25	30	25	187	20	—	200
Terminals 51 / 52												

All outputs are electrically isolated from each other and from the power supply.

Digital outputs DO1 / DO2 are not electrically isolated from each other. Terminals 42 / 52 have the same potential.

Special connection conditions

Note

If the protective earth (PE) is connected in the flowmeter's terminal box, you must ensure that no dangerous potential difference can arise between the protective earth (PE) and the potential equalization (PA) in areas with explosion risk.

Note

The safety requirements for intrinsically safe circuits in the EC type examination certificate of the device must be complied with.

The output circuits are designed so that they can be connected to both intrinsically-safe and non-intrinsically-safe circuits.

- Combining intrinsically safe and non-intrinsically safe circuits is not permitted.
- On intrinsically safe circuits, potential equalization should be established along the entire length of the cable used for the signal outputs.
- The rated voltage of the non-intrinsically safe circuits is U_M = 30 V.
- Intrinsic safety is preserved if the rated voltage U_M = 30 V is not up-scaled when connections are established to non-intrinsically safe external circuits.
- When changing the type of protection, the information in the corresponding chapter **Changing the type of protection** in operating instruction must be observed.

Use in hazardous areas in accordance with EAC TR-CU-012

Note

- An additional document with information on EAC-Ex certification is available for measuring systems that are used in potentially explosive atmospheres in accordance with EAC TR-CU-012.
- The information on EAC-Ex certification is an integral part of this instruction. As a result, it is crucial that the installation guidelines and connection values it lists are also observed.

The icon on the name plate indicates the following:



Information on EAC-Ex certification is available for free download at the following link. Alternatively simply scan the QR code.



[INF/FCX100/FCX400/EAC-Ex-X8](#)

Questionnaire

Customer:	Date:
Ms. / Mr.:	Department:
Telephone:	Fax:

Measuring medium	Liquid content:	Gas content:
Flow rate: (min., max., operating point)	kg/h	
Density: (min., max., operating point)	kg/m ³	
Dynamic viscosity: (min., max., operating point)	mPas/cP	
Measuring medium temperature: (min., max., operating point)	°C	
Ambient temperature	°C	
Pressure: (min., max., operating point)	bar	
Rate of flow:	<input type="checkbox"/> Steady	<input type="checkbox"/> Pulsating
Batch operation:	<input type="checkbox"/> Yes	<input type="checkbox"/> No
Concentration calculation:	<input type="checkbox"/> Yes	<input type="checkbox"/> No
Transmitter design:	<input type="checkbox"/> Integral mount design	<input type="checkbox"/> Remote mount design
Explosion protection:	<input type="checkbox"/> Yes	<input type="checkbox"/> No
Power supply:	<input type="checkbox"/> 11 to 30 V DC	
Electrical outputs:	Communication:	
	<input type="checkbox"/> Pulse output, passive	<input type="checkbox"/> Modbus-RTU, RS 485
Additional specifications:		
Pipeline diameter:mm	
Process connection:	

Trademarks

Modbus is a registered trademark of Schneider Automation Inc.

Hastelloy C-4 is a trademark of Haynes International

Hastelloy C-22 is a trademark of Haynes International

Windows is a registered trademark of Microsoft Corporation.

Sales



Service



ABB Measurement & Analytics

For your local ABB contact, visit:

www.abb.com/contacts

For more product information, visit:

www.abb.com/flow

We reserve the right to make technical changes or modify the contents of this document without prior notice. With regard to purchase orders, the agreed particulars shall prevail.
ABB does not accept any responsibility whatsoever for potential errors or possible lack of information in this document.

We reserve all rights in this document and in the subject matter and illustrations contained therein.
Any reproduction, disclosure to third parties or utilization of its contents – in whole or in parts – is forbidden without prior written consent of ABB.